

Sample Name :Bid BH3 Peptide
 Cat No :RP20440
 Lot No :E6059520K
 Time Processed :16:23:06
 Month-Day-Year Processed :11/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

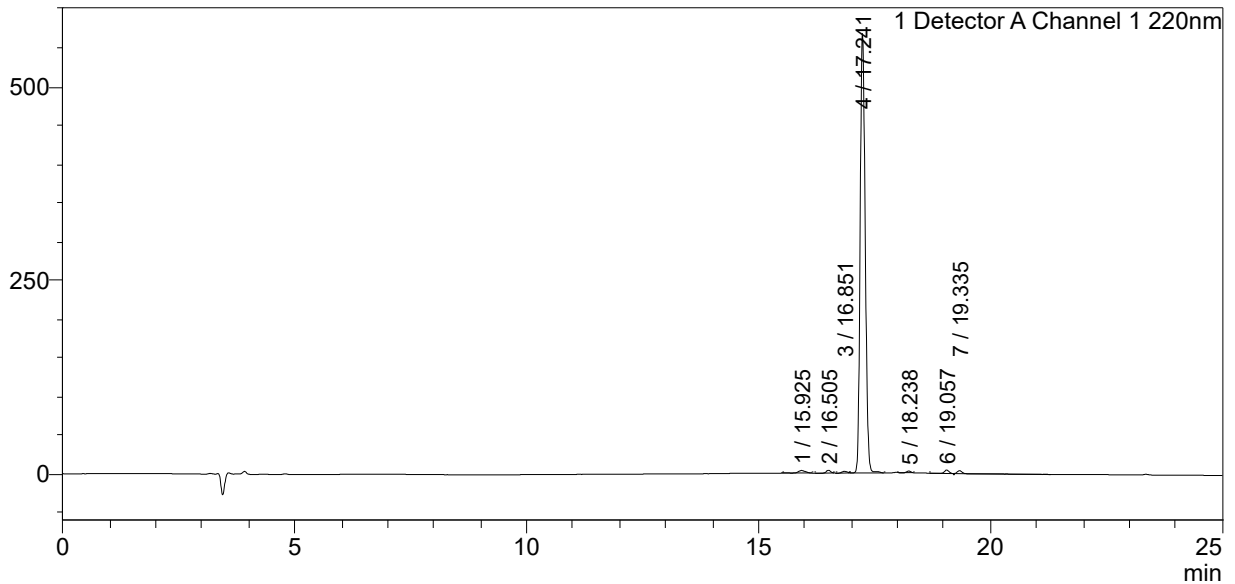

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.925	35282	3332	0.803
2	16.505	22249	3642	0.506
3	16.851	16512	2205	0.376
4	17.241	4267004	567312	97.105
5	18.238	8360	2011	0.190
6	19.057	30194	4404	0.687
7	19.335	14594	3779	0.332
Total		4394194	586686	100.000