

Sample Name: Arg-Gly-Asp-Cys
 Cat No. : RP10860
 Lot No. : E4052519K
 Time Processed: 2:44:49 PM
 Month-Day-Year Processed :11/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

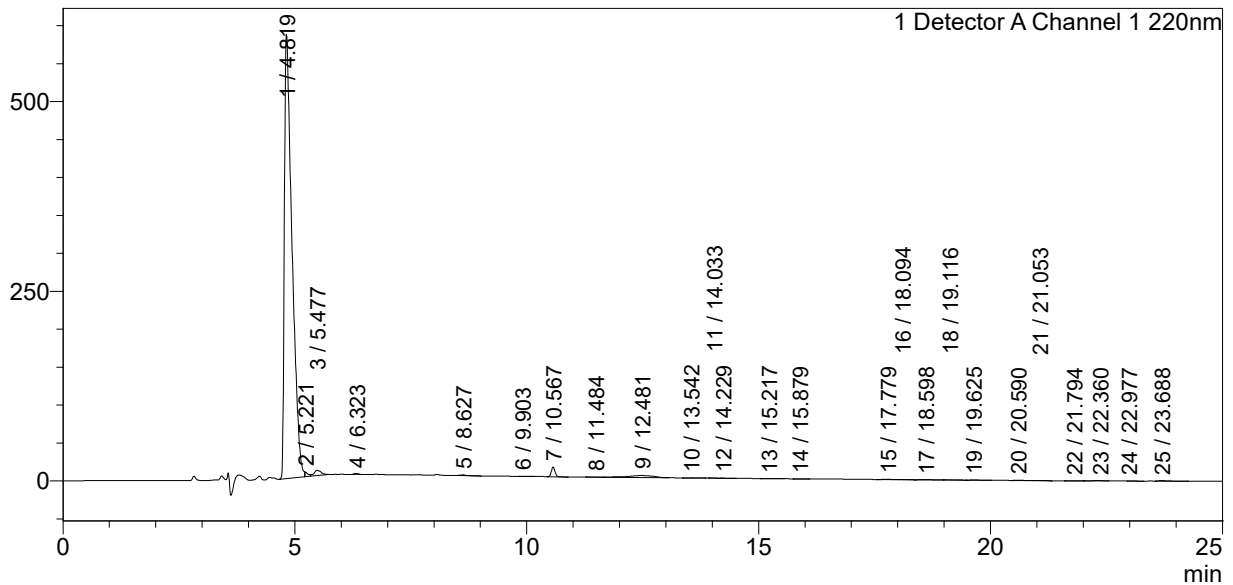

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.819	6714188	585734	95.078
2	5.221	26277	6358	0.372
3	5.477	72886	6852	1.032
4	6.323	5398	1084	0.076
5	8.627	6082	830	0.086
6	9.903	1024	61	0.015
7	10.567	70605	12779	1.000
8	11.484	6029	369	0.085
9	12.481	107421	2662	1.521
10	13.542	2976	184	0.042
11	14.033	1434	248	0.020
12	14.229	1159	120	0.016
13	15.217	3898	194	0.055
14	15.879	1046	117	0.015

Peak#	Ret. Time	Area	Height	Area%
15	17.779	2222	164	0.031
16	18.094	1164	89	0.016
17	18.598	4190	203	0.059
18	19.116	4069	212	0.058
19	19.625	3956	259	0.056
20	20.590	4089	269	0.058
21	21.053	2162	189	0.031
22	21.794	1439	116	0.020
23	22.360	8282	710	0.117
24	22.977	1150	107	0.016
25	23.688	8656	882	0.123
Total		7061802	620791	100.000