

Sample Name : Arg-Gly-Asp-Ser
 Cat No. : RP10861
 Lot No. : E7491421B
 Time Processed : 21:10:44
 Month-Day-Year Processed : 02/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

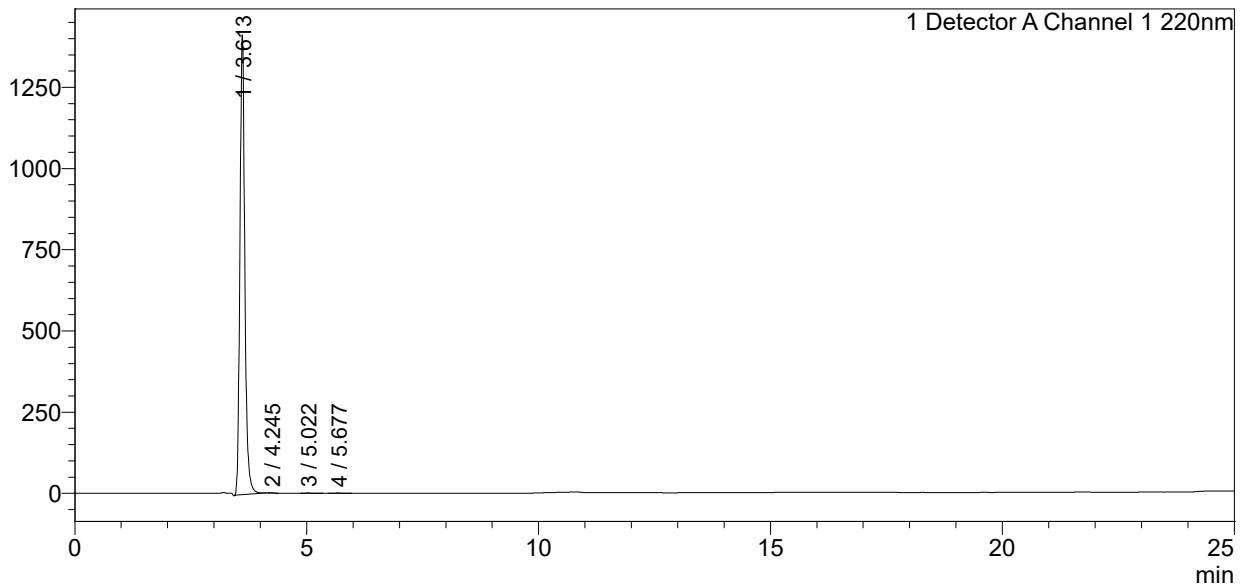

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	3.613	10354287	1415949	99.788
2	4.245	6776	1253	0.065
3	5.022	7233	1030	0.070
4	5.677	8007	1023	0.077
Total		10376302	1419255	100.000