


Mass Spectrum

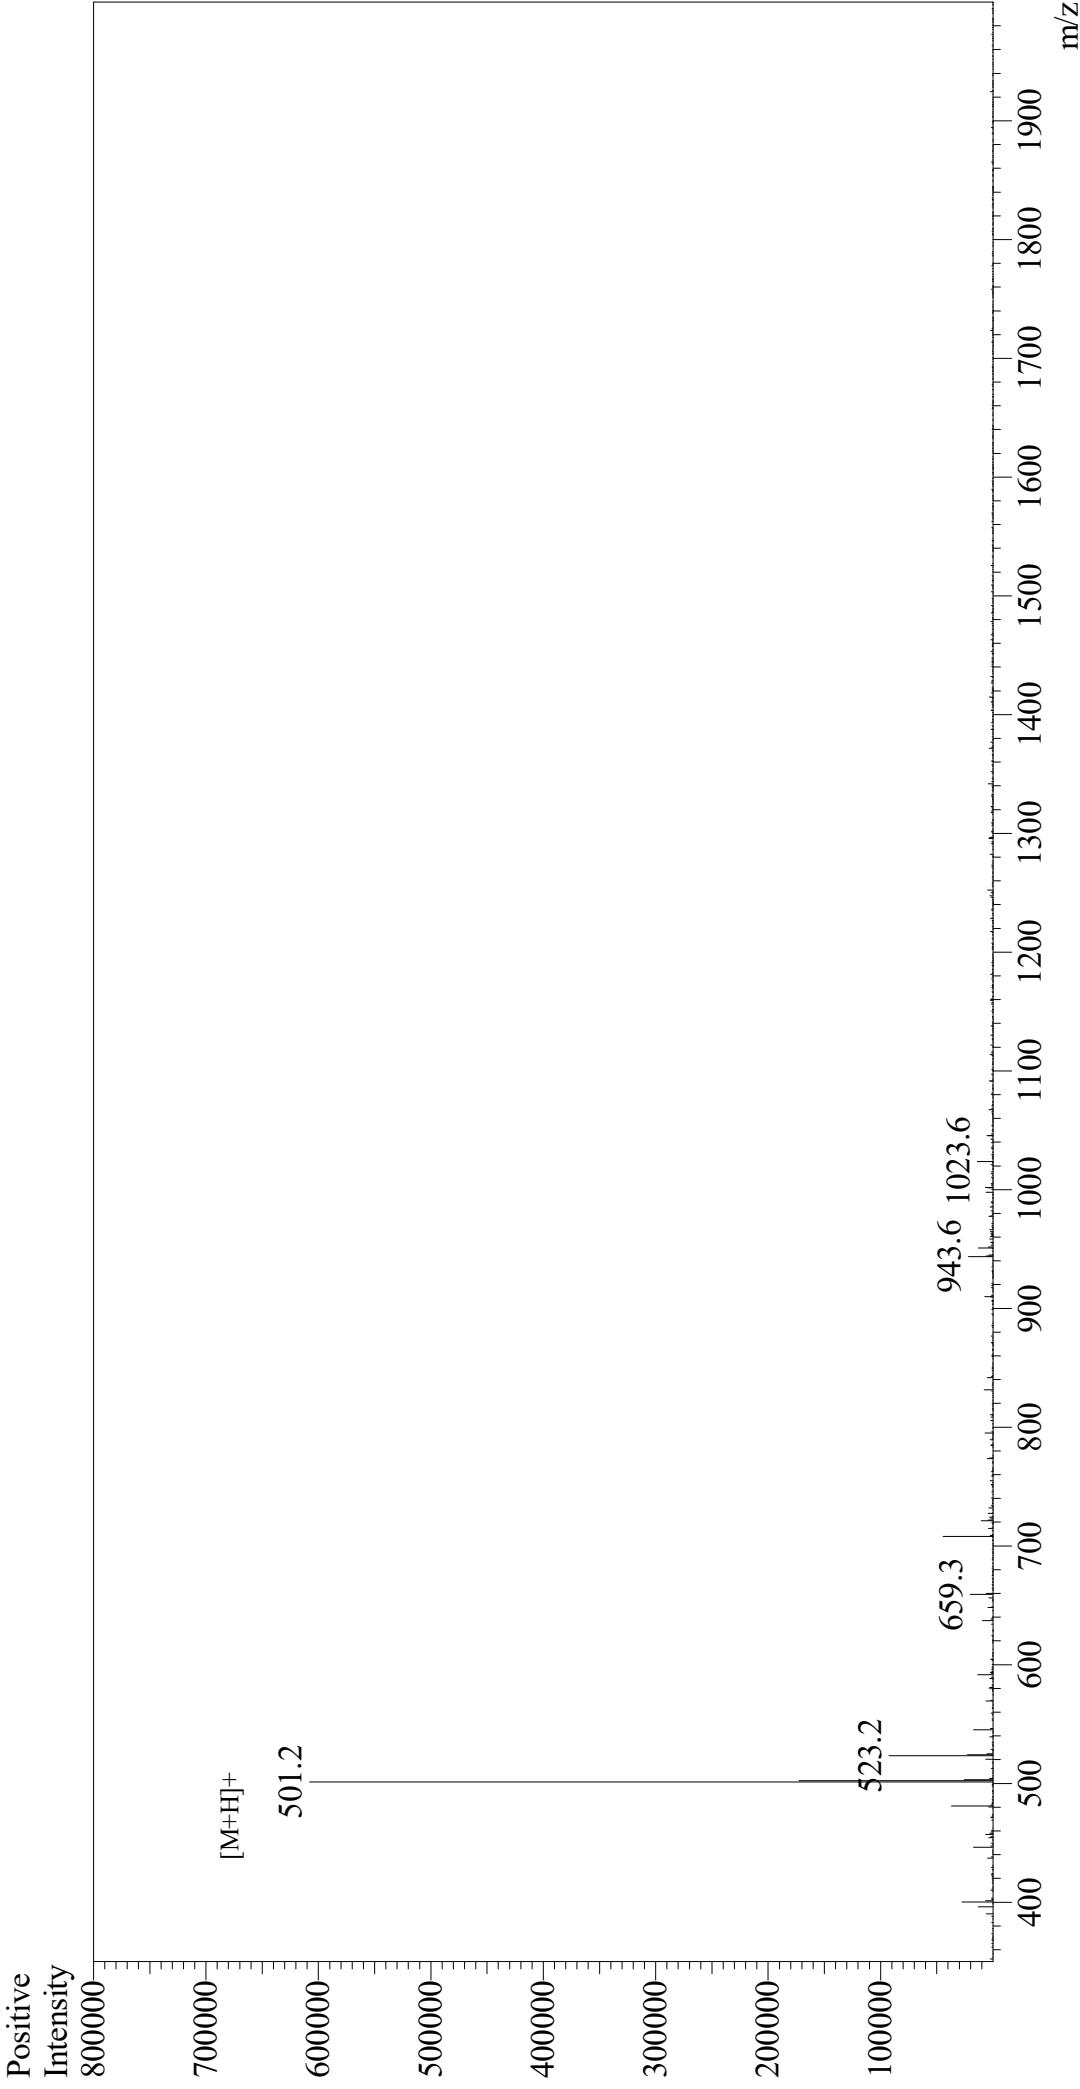

Sample Information
Month-Day Processed : 05/26/21
Time Processed : 7:59:15 AM
Injection Volume : 0.2
Sample Name : Tuftsin
Cat No : RP10624
Lot No : E6951221E
Theoretical MW : 500.60
Observed MW : 500.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH