

Sample Name : α -MSH, amide
 Cat. No.: RP10644
 Lot. No. :PE6141901
 Time Processed :17:28:06
 Month-Day-Year Processed :01/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

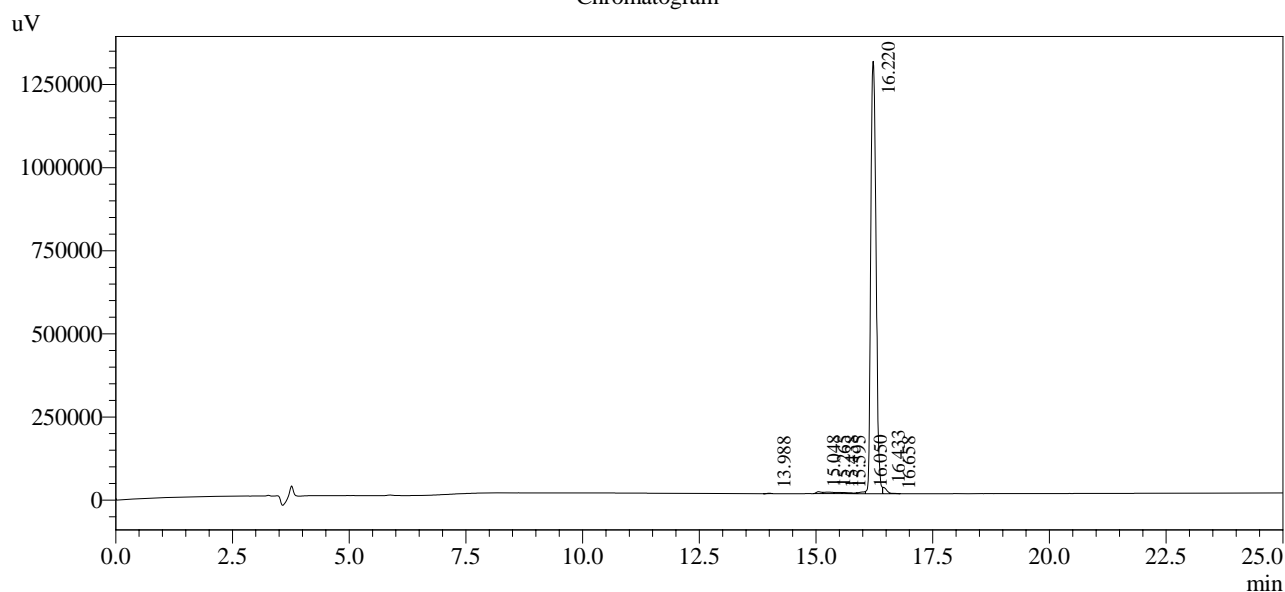

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.988	6763	1280	0.064
2	15.048	46656	5853	0.440
3	15.265	61786	4630	0.583
4	15.438	38266	3839	0.361
5	15.595	51761	3428	0.488
6	16.050	49139	6081	0.464
7	16.220	10228408	1300592	96.520
8	16.433	108878	19048	1.027
9	16.658	5485	968	0.052
Total		10597142	1345718	100.000