

Sample Name :43Gap 26, Connexin Mimetic
 Cat. No. : RP20274
 Lot. No. :E7770819F
 Time Processed : 10:23:38
 Month-Day-Year Processed : 06/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

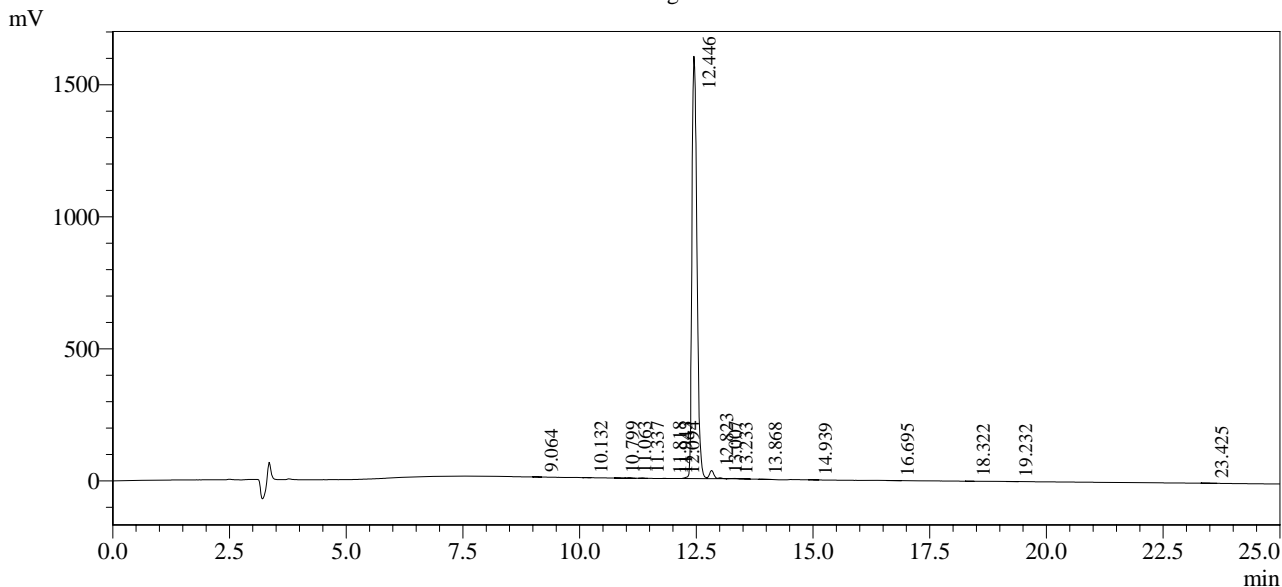

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.064	3463	715	0.028
2	10.132	1748	364	0.014
3	10.799	1425	192	0.012
4	11.063	9134	1628	0.074
5	11.337	5954	1200	0.048
6	11.818	3869	694	0.031
7	11.943	1786	316	0.015
8	12.094	3289	489	0.027
9	12.446	12022964	1599448	97.706
10	12.823	200224	30807	1.627
11	13.007	16315	3365	0.133
12	13.233	12912	653	0.105
13	13.868	2164	217	0.018
14	14.939	1511	248	0.012
15	16.695	7628	834	0.062
16	18.322	1440	286	0.012
17	19.232	5560	953	0.045
18	23.425	3866	434	0.031
Total		12305252	1642844	100.000