

Sample Name : CEF14, EBV Rta Protein (28-37)
 Cat. No. : RP20442
 Lot. No. : E7081319J
 Time Processed :21:43:51
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	20	
25.00	Pumps	Pump A B.Conc	80	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	20	
40.00	Pumps	Pump A B.Conc	20	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

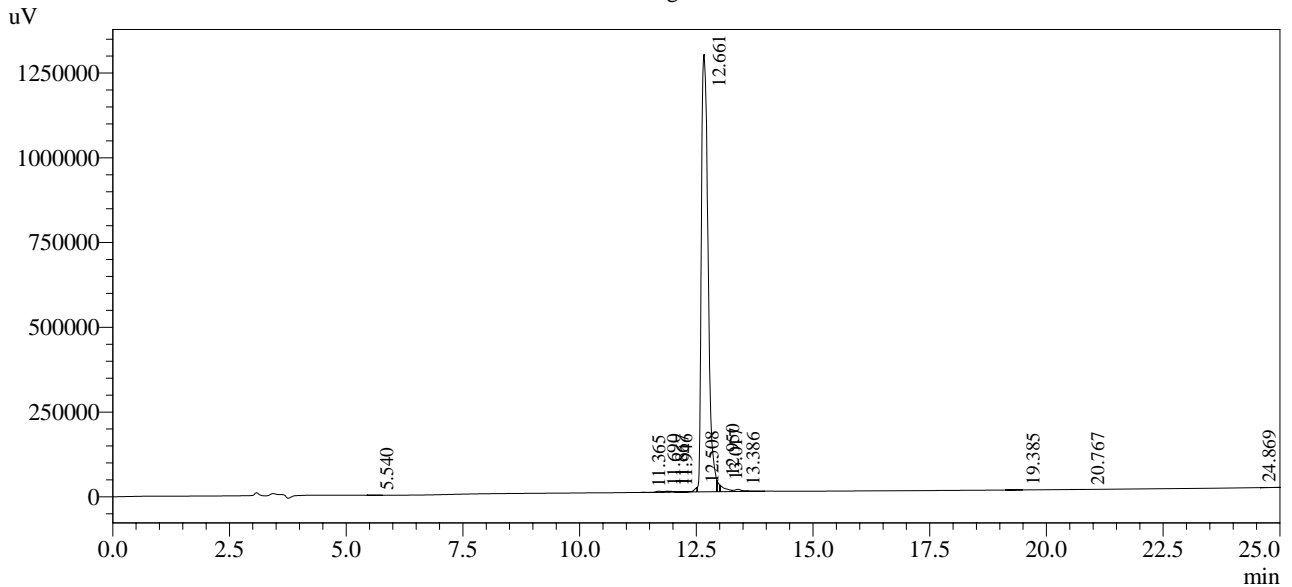

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.540	1299	134	0.010
2	11.365	5591	722	0.042
3	11.690	28757	3470	0.215
4	11.867	18129	2886	0.135
5	11.946	16963	2685	0.127
6	12.508	55734	12369	0.416
7	12.661	12940393	1290880	96.590
8	12.950	98002	30706	0.732
9	13.017	137355	18670	1.025
10	13.386	83424	6374	0.623
11	19.385	2009	223	0.015
12	20.767	1010	38	0.008
13	24.869	8538	882	0.064
Total		13397204	1370039	100.000