

Sample Name : [Glu1]-Fibrinopeptide B
Cat. No. : RP20439
Lot. No. : E9911121F
Time Processed : 12:54:27
Month-Day-Year Processed : 06/16/2021
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow: 1 ml/min
Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ19010140

<Chromatogram>

mV

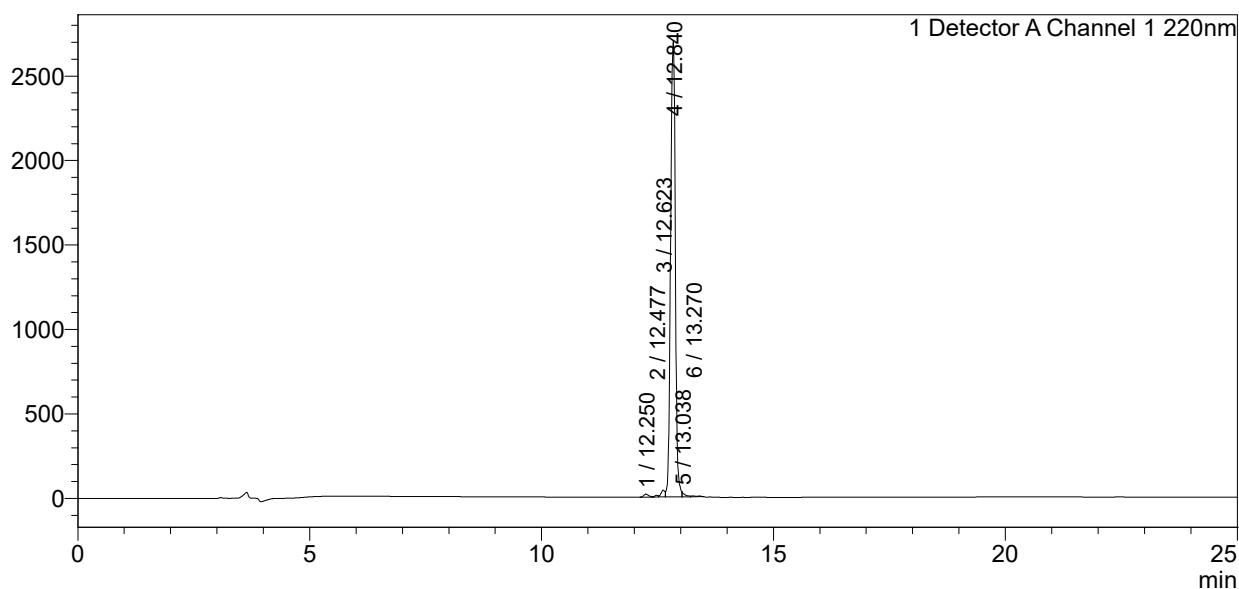

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.250	131372	17913	0.659
2	12.477	52372	10071	0.263
3	12.623	231493	40249	1.161
4	12.840	19355765	2701597	97.069
5	13.038	119747	25726	0.601
6	13.270	49536	4975	0.248
Total		19940286	2800531	100.000