

Sample Name : Bradykinin  
 Cat. No. : RP11129  
 Lot. No. : E6264419H  
 Time Processed :6:21:32  
 Month-Day-Year Processed :08/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010009

Chromatogram

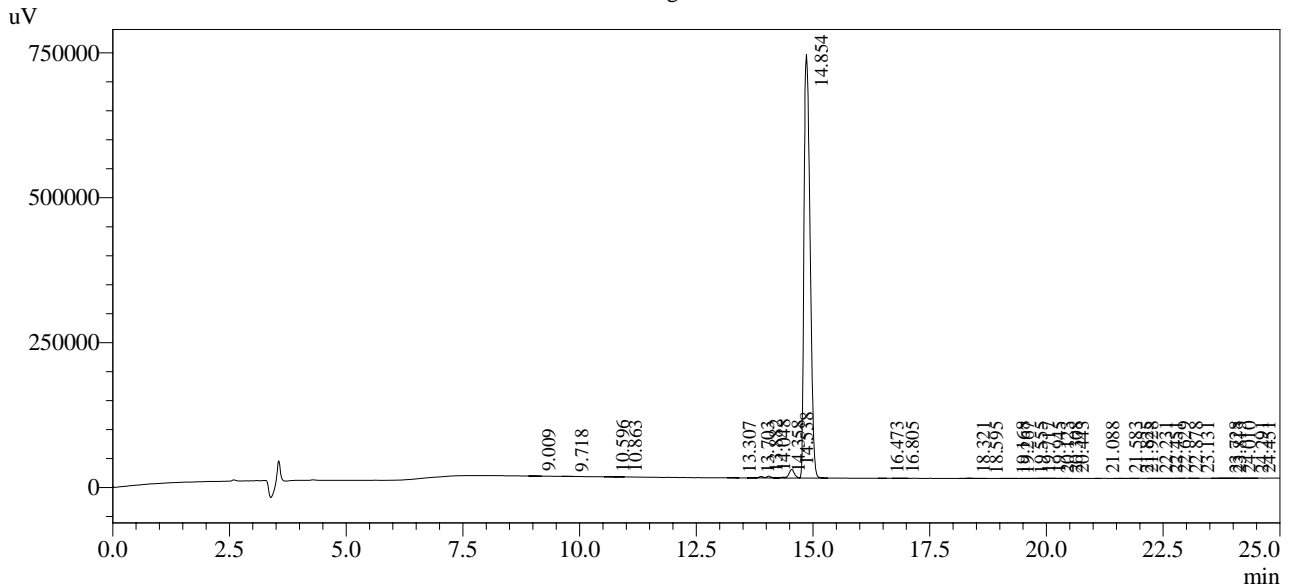

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.009	1607	174	0.024
2	9.718	2262	234	0.033
3	10.596	1051	165	0.015
4	10.863	1027	188	0.015
5	13.307	1477	212	0.022
6	13.703	1236	166	0.018
7	13.882	17294	2698	0.254
8	14.048	20947	3222	0.307
9	14.358	9365	1420	0.137
10	14.538	118590	14821	1.738
11	14.854	6596740	731322	96.700
12	16.473	1019	154	0.015
13	16.805	2402	204	0.035
14	18.321	5886	563	0.086
15	18.595	1636	202	0.024
16	19.168	1875	205	0.027
17	19.267	1258	193	0.018
18	19.555	1243	229	0.018
19	19.717	1725	236	0.025
20	19.945	3819	320	0.056
21	20.123	3425	317	0.050
22	20.308	1518	226	0.022
23	20.443	1445	255	0.021
24	21.088	1145	188	0.017

Peak#	Ret. Time	Area	Height	Area %
25	21.583	1195	166	0.018
26	21.825	2348	305	0.034
27	21.928	1190	291	0.017
28	22.231	1215	190	0.018
29	22.451	1937	233	0.028
30	22.629	1264	162	0.019
31	22.878	2086	265	0.031
32	23.131	1528	197	0.022
33	23.728	2086	260	0.031
34	23.813	2076	335	0.030
35	24.010	1407	192	0.021
36	24.291	2541	256	0.037
37	24.451	1017	135	0.015
Total		6821880	760899	100.000