

Sample Name:[Met5]-Enkephalin
 Cat No. :RP10886
 Lot No. :E9006920G
 Time Processed :3:33:46 PM
 Month-Day-Year Processed :07/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

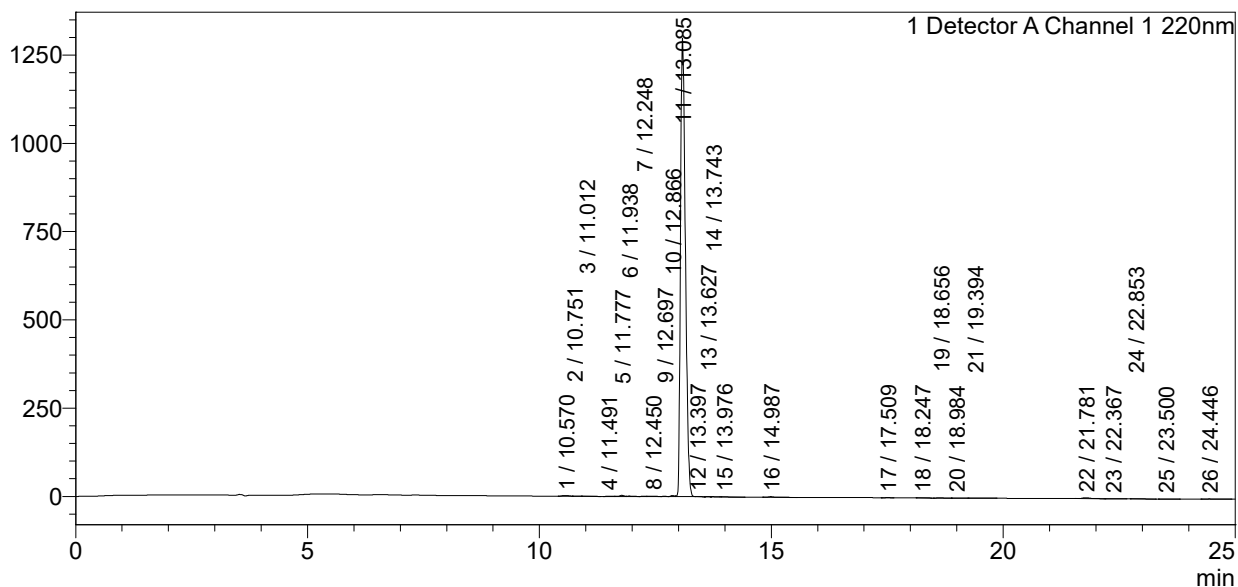

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.570	21387	2153	0.219
2	10.751	4146	624	0.042
3	11.012	5092	330	0.052
4	11.491	5281	702	0.054
5	11.777	20830	3010	0.213
6	11.938	9823	1175	0.101
7	12.248	3330	408	0.034
8	12.450	8987	988	0.092
9	12.697	5047	1074	0.052
10	12.866	18389	3179	0.188
11	13.085	9563689	1298888	97.939
12	13.397	3197	455	0.033
13	13.627	4610	910	0.047
14	13.743	4252	704	0.044
15	13.976	2741	143	0.028

Peak#	Ret. Time	Area	Height	Area%
16	14.987	19588	1931	0.201
17	17.509	3642	481	0.037
18	18.247	3030	283	0.031
19	18.656	2048	185	0.021
20	18.984	1416	116	0.014
21	19.394	3786	240	0.039
22	21.781	30511	2684	0.312
23	22.367	4769	353	0.049
24	22.853	2853	112	0.029
25	23.500	3104	278	0.032
26	24.446	9382	761	0.096
Total		9764929	1322167	100.000