

Sample Name :Angiotensin II, human
 Cat No :RP11257
 Lot No :E7878120L
 Time Processed :21:09:35
 Month-Day-Year Processed :12/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

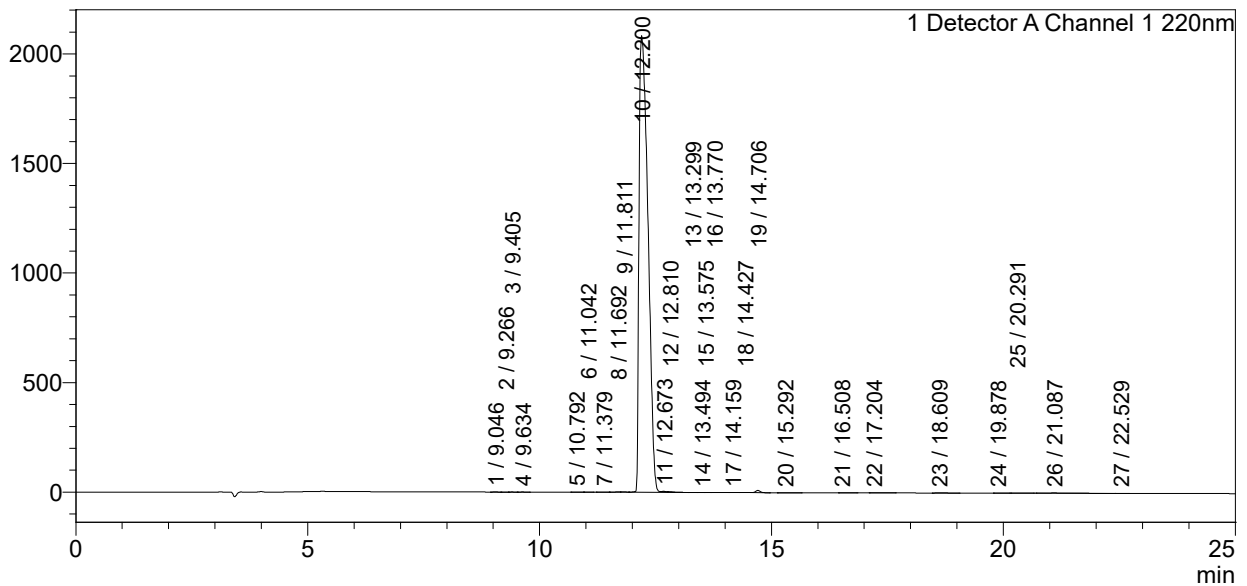

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.046	3239	564	0.012
2	9.266	1319	210	0.005
3	9.405	2275	381	0.008
4	9.634	3396	529	0.012
5	10.792	6441	875	0.023
6	11.042	1954	284	0.007
7	11.379	3476	555	0.012
8	11.692	16841	2283	0.060
9	11.811	17632	2433	0.063
10	12.200	27838135	2085213	99.174
11	12.673	9993	2111	0.036
12	12.810	4267	941	0.015
13	13.299	2141	392	0.008
14	13.494	3135	493	0.011
15	13.575	3151	515	0.011
16	13.770	3925	352	0.014

Peak#	Ret. Time	Area	Height	Area%
17	14.159	1194	207	0.004
18	14.427	2428	262	0.009
19	14.706	71048	10375	0.253
20	15.292	2086	114	0.007
21	16.508	1478	122	0.005
22	17.204	4028	365	0.014
23	18.609	8689	670	0.031
24	19.878	1412	100	0.005
25	20.291	2531	131	0.009
26	21.087	50341	1703	0.179
27	22.529	3551	449	0.013
Total		28070106	2112629	100.000