

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : E5545319H
 Time Processed :7:58:25 AM
 Month-Day-Year Processed :08/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

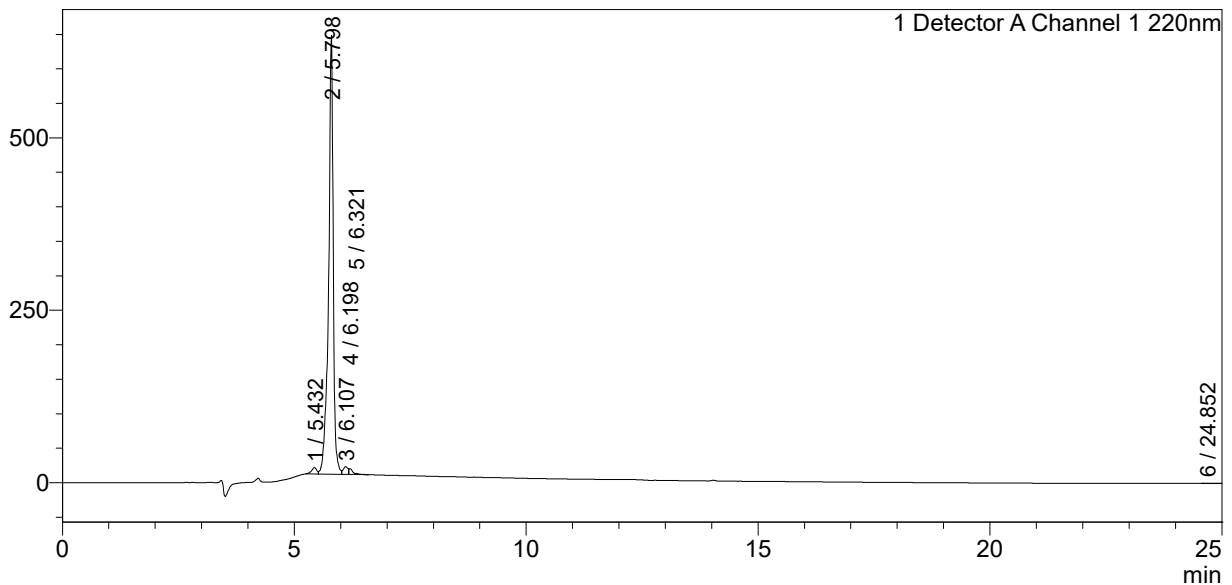

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.432	68302	9145	1.462
2	5.798	4470378	636212	95.666
3	6.107	79639	11031	1.704
4	6.198	41506	8206	0.888
5	6.321	10064	1589	0.215
6	24.852	3034	278	0.065
Total		4672924	666461	100.000