

Sample Name :Hexa-His  
 Cat No. :RP11737  
 Lot No. :E8043421E  
 Time Processed : 4:43:05 PM  
 Month-Day-Year Processed : 05/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010017

mV

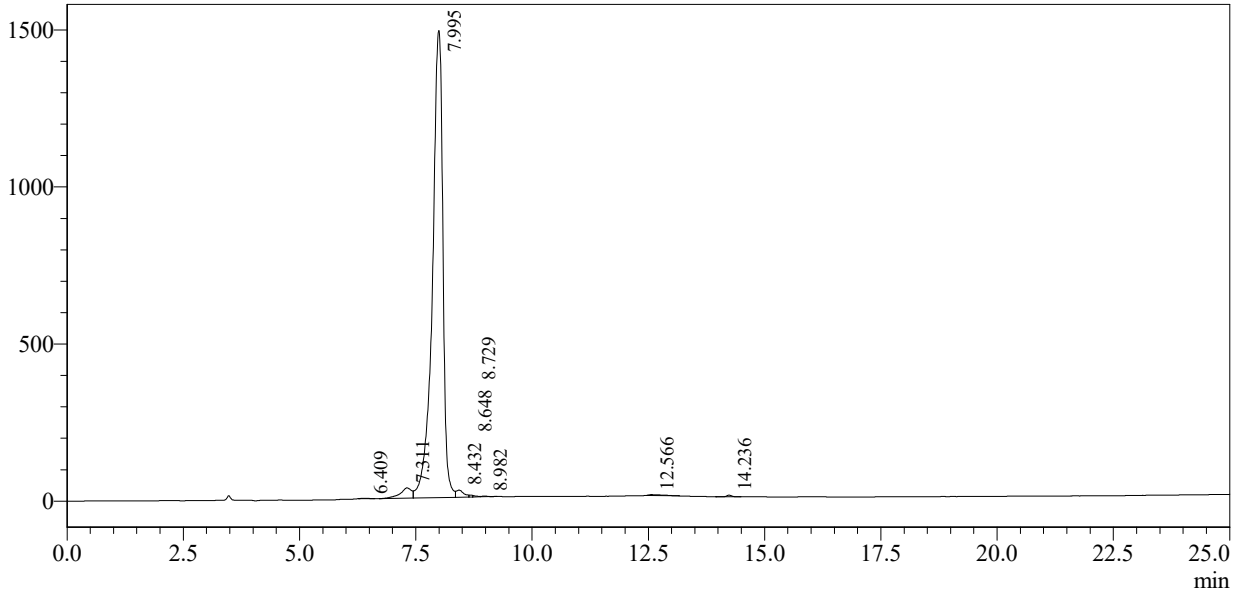

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.409	14357	1314	0.059
2	7.311	560350	32729	2.310
3	7.995	23267703	1486080	95.899
4	8.432	257636	22489	1.062
5	8.648	29537	6435	0.122
6	8.729	24511	4861	0.101
7	8.982	17892	1954	0.074
8	12.566	55238	2502	0.228
9	14.236	35530	5166	0.146
Total		24262755	1563531	100.000