

Sample Name :HPV16-E711-20 epitope
 Cat No. :RP20285
 Lot No. :E4869619I
 Time Processed :10:29:38
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

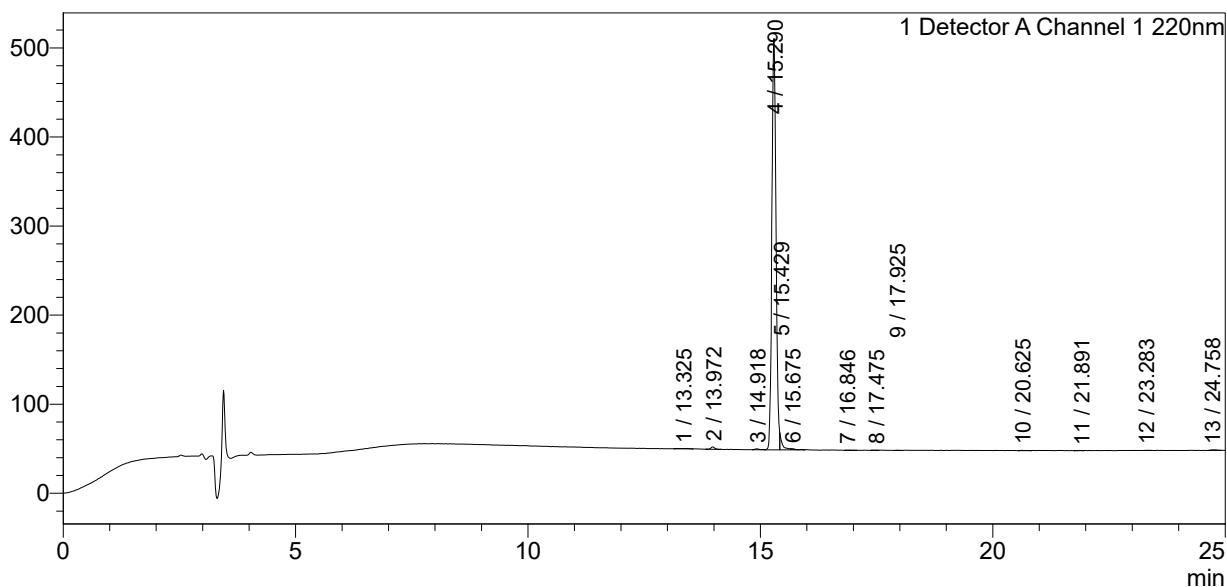

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.325	4514	332	0.154
2	13.972	15197	2652	0.517
3	14.918	7340	1017	0.250
4	15.290	2830176	461695	96.254
5	15.429	64758	16218	2.202
6	15.675	1302	273	0.044
7	16.846	1980	215	0.067
8	17.475	1263	203	0.043
9	17.925	1417	254	0.048
10	20.625	2720	290	0.093
11	21.891	2041	259	0.069
12	23.283	1963	179	0.067
13	24.758	5644	634	0.192
Total		2940317	484221	100.000