

Sample Name :Glucagon-Like Peptide (GLP) II, human
 Cat No. :RP10769
 Lot No. :PE2051903
 Time Processed :9:14:47
 Month-Day-Year Processed :03/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

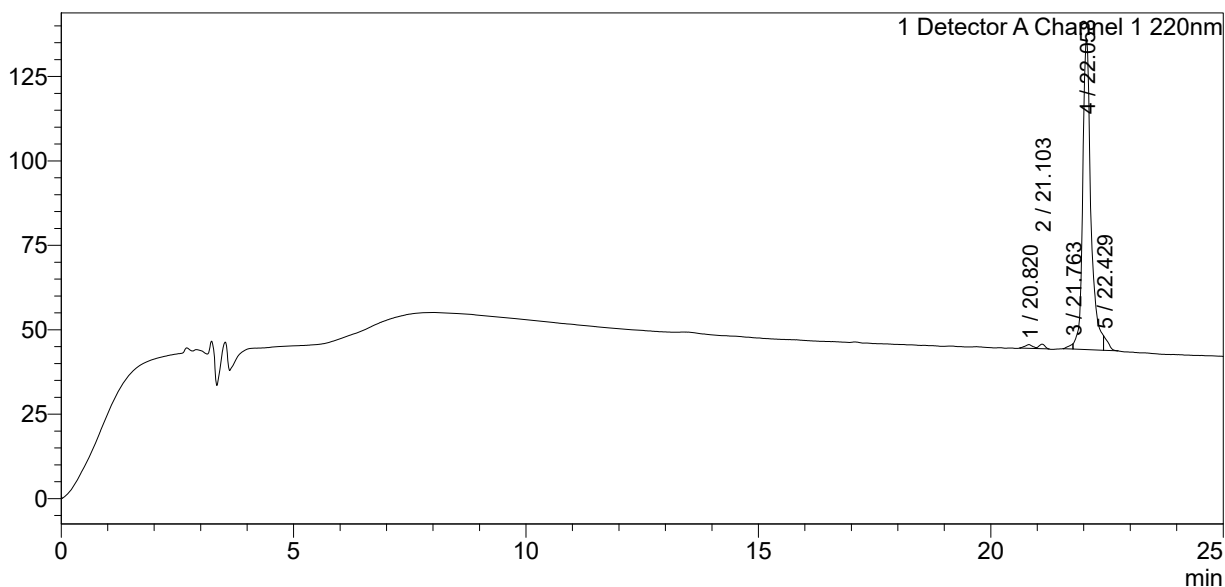

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	20.820	12331	1096	1.033
2	21.103	11577	1338	0.970
3	21.763	9068	1426	0.760
4	22.058	1134368	92104	95.010
5	22.429	26596	4339	2.228
Total		1193941	100302	100.000