

Sample Name :Crosstide
 Cat No :RP20200
 Lot No :E7123721A
 Time Processed :19:32:00
 Month-Day-Year Processed :01/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

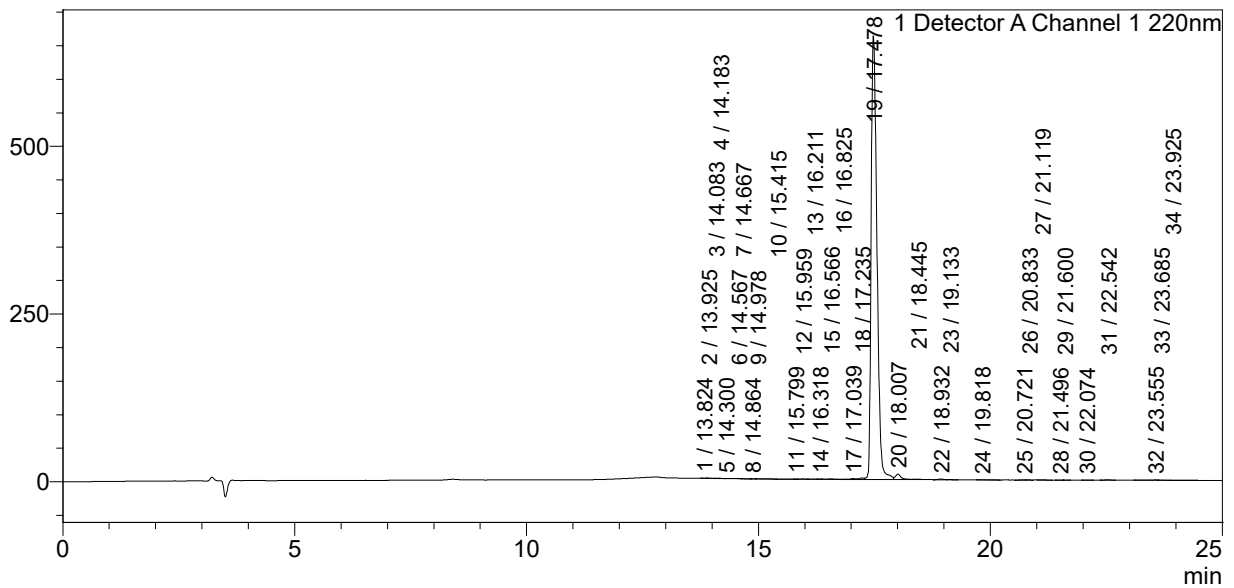

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.824	568	80	0.010
2	13.925	1261	143	0.021
3	14.083	691	126	0.012
4	14.183	1166	178	0.020
5	14.300	1878	178	0.032
6	14.567	261	70	0.004
7	14.667	319	70	0.005
8	14.864	218	61	0.004
9	14.978	839	74	0.014
10	15.415	602	62	0.010
11	15.799	53	20	0.001
12	15.959	3460	561	0.059
13	16.211	958	111	0.016
14	16.318	546	126	0.009
15	16.566	7828	819	0.132

Peak#	Ret. Time	Area	Height	Area%
16	16.825	2971	322	0.050
17	17.039	11461	1244	0.194
18	17.235	14304	2213	0.242
19	17.478	5728627	661670	96.957
20	18.007	70473	8293	1.193
21	18.445	8030	778	0.136
22	18.932	7801	1029	0.132
23	19.133	1463	153	0.025
24	19.818	2184	168	0.037
25	20.721	1364	154	0.023
26	20.833	1026	136	0.017
27	21.119	3866	348	0.065
28	21.496	1536	184	0.026
29	21.600	1290	182	0.022
30	22.074	1742	194	0.029
31	22.542	5579	631	0.094
32	23.555	9245	487	0.156
33	23.685	7193	442	0.122
34	23.925	7616	371	0.129
Total		5908418	681679	100.000