

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E4013321F
 Time Processed :2:16:31 PM
 Month-Day-Year Processed :06/29/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

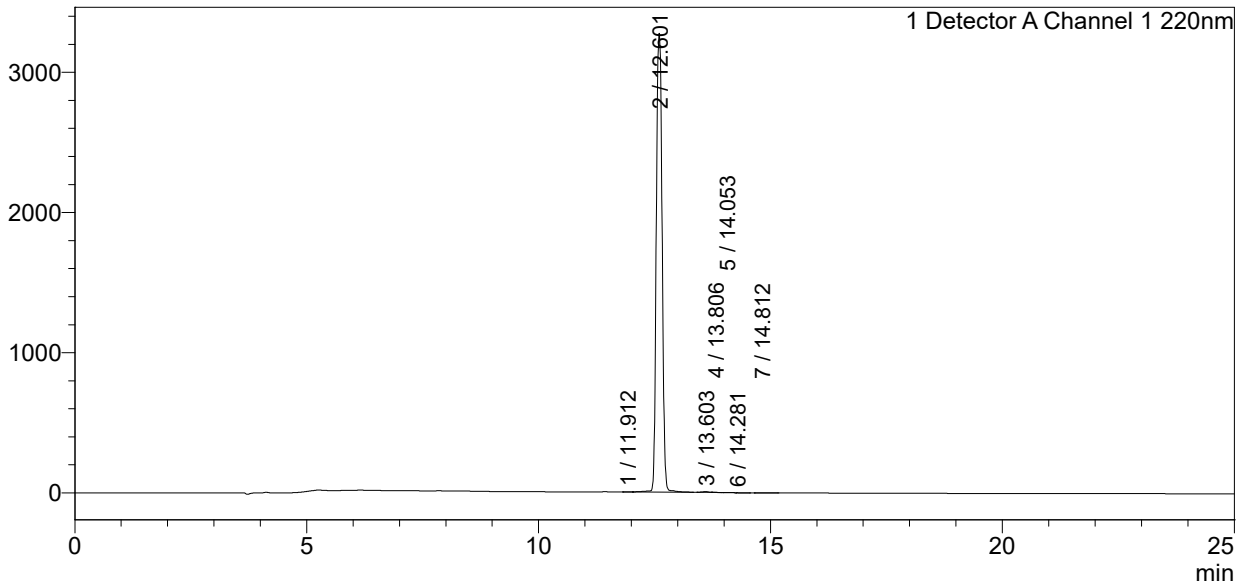

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.912	17871	1879	0.062
2	12.601	28623138	3274610	99.702
3	13.603	47654	5527	0.166
4	13.806	6603	1033	0.023
5	14.053	2455	347	0.009
6	14.281	1776	79	0.006
7	14.812	9266	737	0.032
Total		28708762	3284212	100.000