

Sample Name :Amylin (8-37), amide, rat  
Cat. No. : RP11277  
Lot. No. :E4725119I  
Time Processed :12:57:36  
Month-Day-Year Processed :10/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
31.00	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

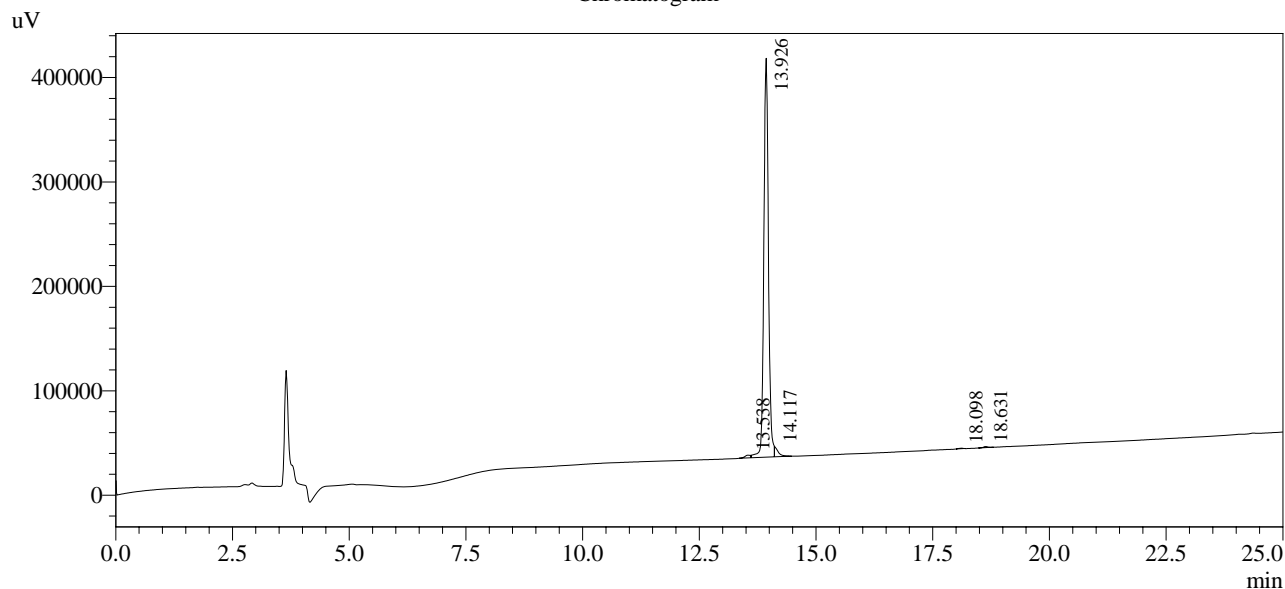

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.538	22909	2691	0.841
2	13.926	2637517	382096	96.856
3	14.117	52385	9685	1.924
4	18.098	3515	549	0.129
5	18.631	6798	1064	0.250
Total		2723123	396086	100.000