

Sample Name : α -MSH, amide
 Cat No. : RP10644
 Lot No. : PE7941902
 Time Processed : 6:31:08
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

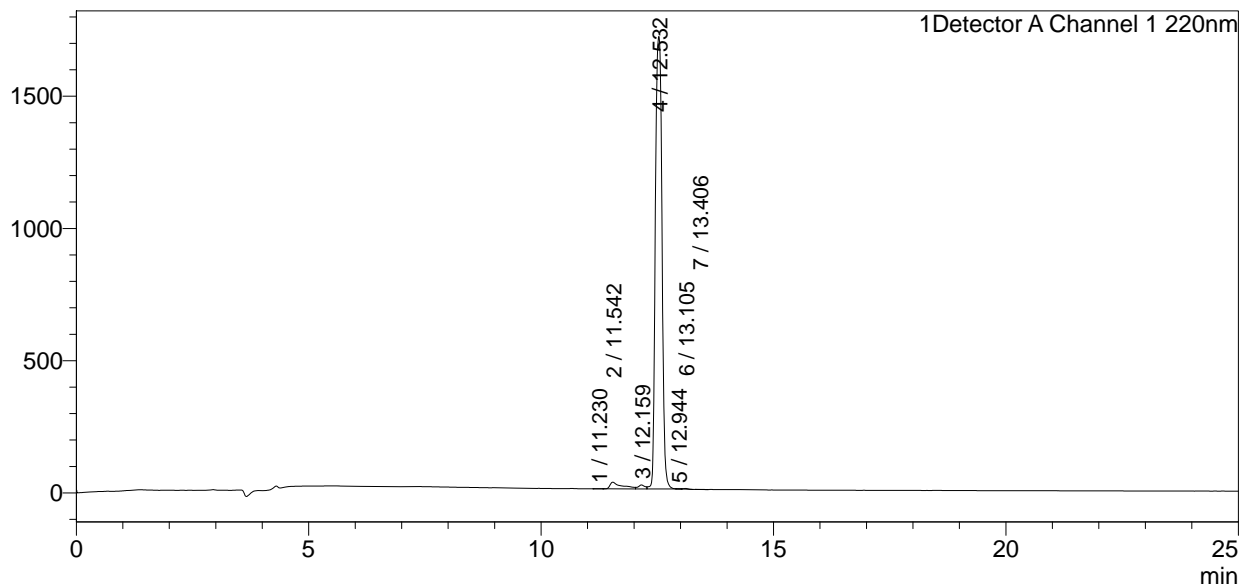

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.230	1950	371	0.011
2	11.542	449847	25189	2.586
3	12.159	148036	15215	0.851
4	12.532	16774415	1710760	96.439
5	12.944	1535	407	0.009
6	13.105	14074	2334	0.081
7	13.406	3887	514	0.022
Total		17393743	1754789	100.000