

Sample Name :Orphanin FQ/Nociceptin, human, mouse, ox, rat  
 Cat No.: RP13084  
 Lot No.:E2811920A  
 Time Processed :4:09:48  
 Month-Day-Year Processed :01/05/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

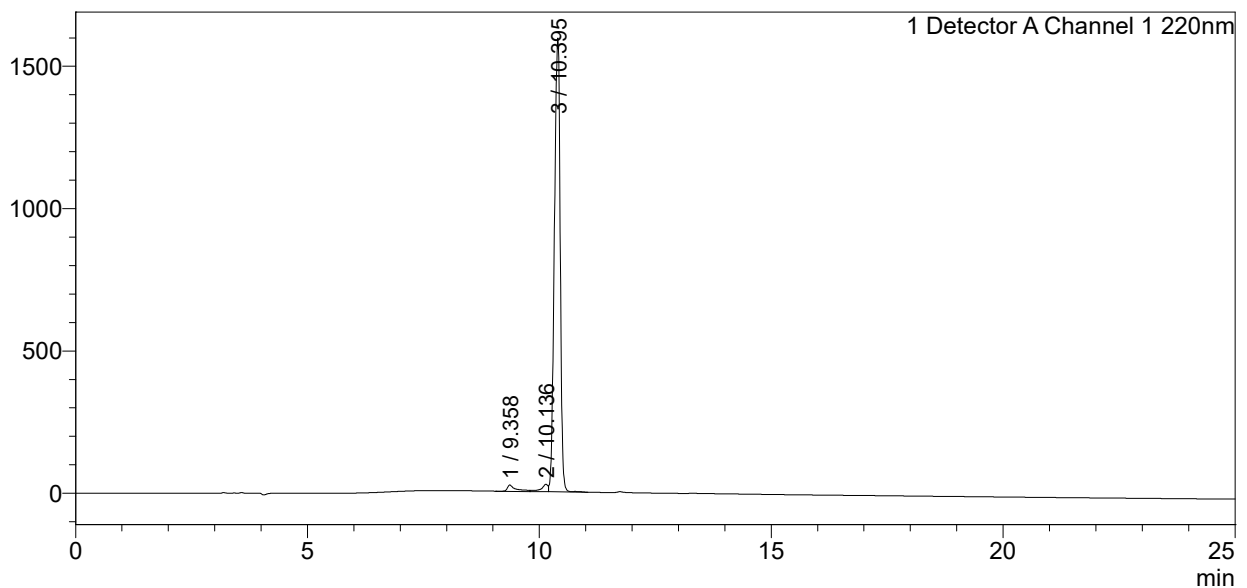

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.358	297739	22343	2.045
2	10.136	276665	26333	1.900
3	10.395	13987192	1594918	96.055
Total		14561595	1643594	100.000