

Sample Name : Neurotensin(8-13)
 Cat. No. : RP10442
 Lot. No. : PE5171707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

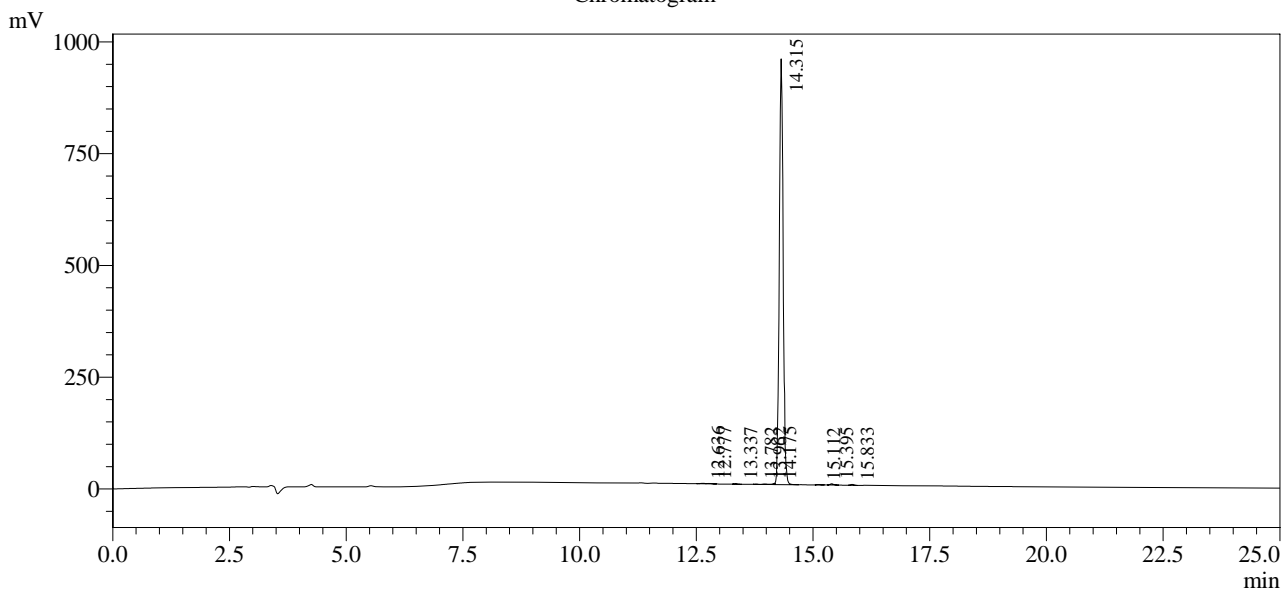

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.636	7423	1097	0.133
2	12.777	6520	1223	0.117
3	13.337	3480	667	0.062
4	13.782	1803	406	0.032
5	13.962	6591	996	0.118
6	14.175	9437	2637	0.169
7	14.315	5507379	952332	98.870
8	15.112	3713	813	0.067
9	15.395	14182	2611	0.255
10	15.833	9808	1922	0.176
Total		5570337	964703	100.000