

Sample Name :Chemerin-9 (149-157)
 Cat No. :RP20248
 Lot No. :E9426021D
 Time Processed :2:12:03 AM
 Month-Day-Year Processed :04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

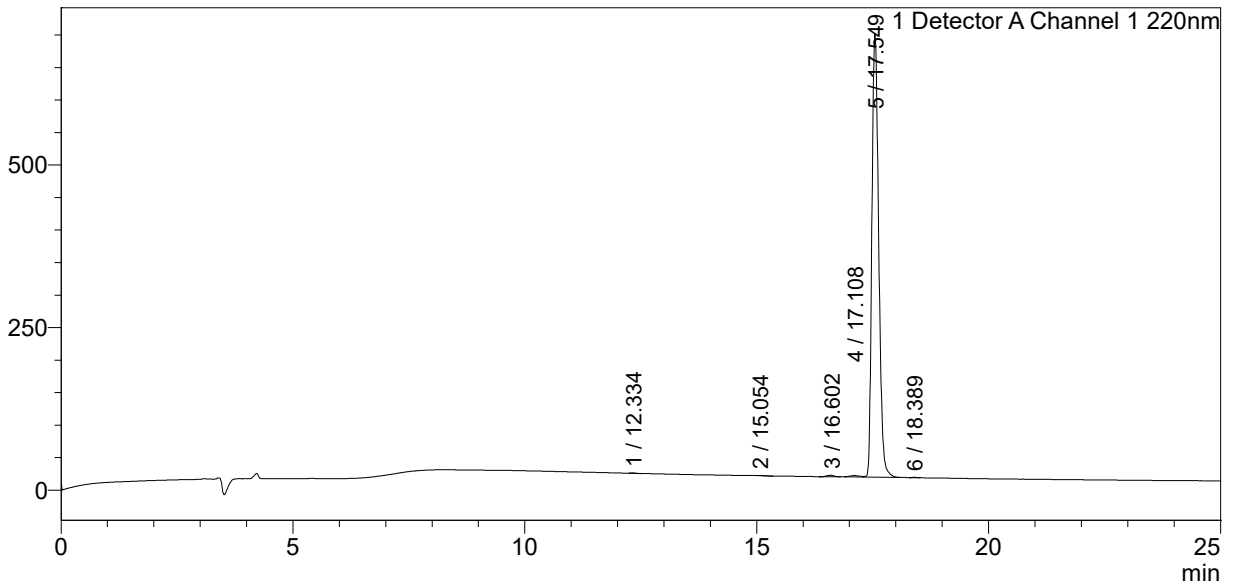

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.334	3907	775	0.056
2	15.054	3712	448	0.053
3	16.602	22125	2144	0.315
4	17.108	27983	1930	0.399
5	17.549	6953923	682309	99.110
6	18.389	4683	751	0.067
Total		7016333	688357	100.000