

Sample Name :TAT
 Cat No. : RP12784
 Lot No. : E9799120J
 Time Processed :1:23:55 AM
 Month-Day-Year Processed :11/10/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GR11010440

<Chromatogram>

mV

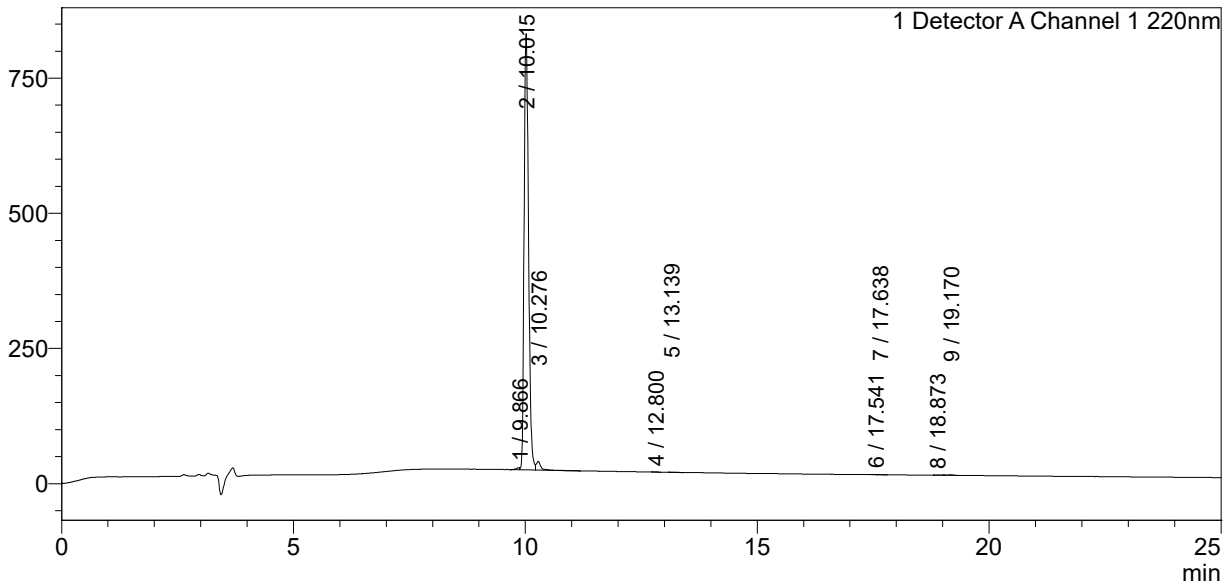

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.866	21510	3967	0.390
2	10.015	5355160	807087	97.198
3	10.276	115504	16085	2.096
4	12.800	1268	273	0.023
5	13.139	1392	155	0.025
6	17.541	3113	511	0.057
7	17.638	2132	405	0.039
8	18.873	1188	158	0.022
9	19.170	8277	1255	0.150
Total		5509543	829898	100.000