

Sample Name : $\beta$ -Amyloid (1-40)  
 Cat No :RP10004  
 Lot No :E0665521A  
 Time Processed :21:41:02  
 Month-Day-Year Processed :04/09/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

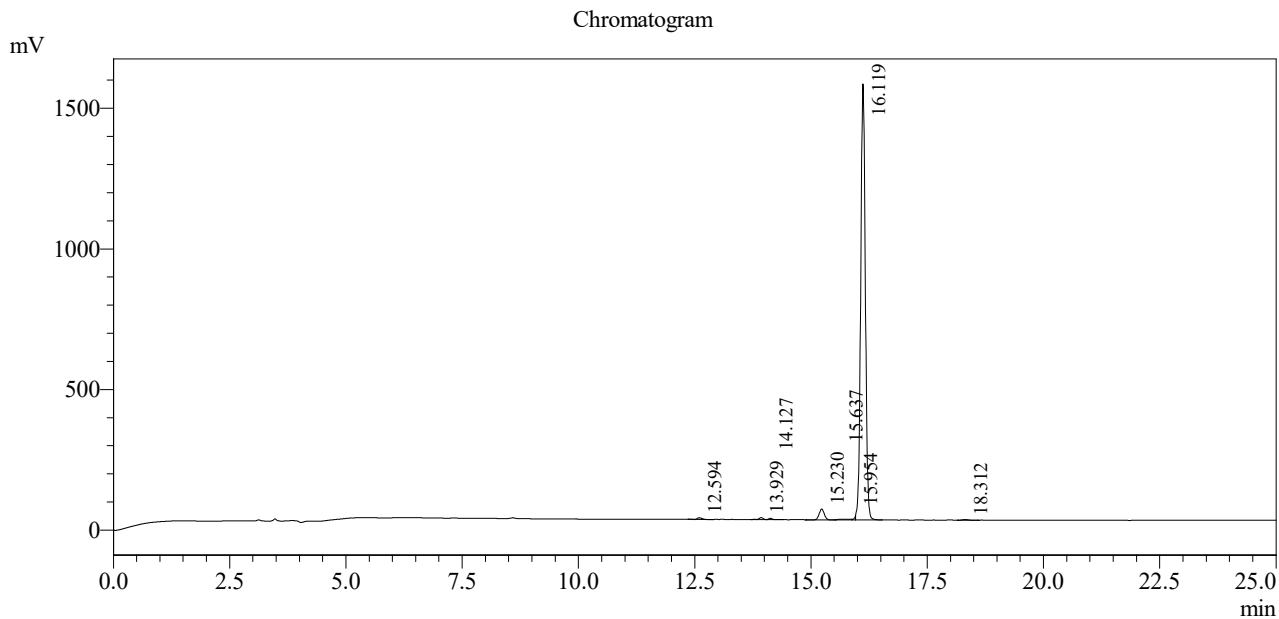

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.594	41122	5905	0.365
2	13.929	46399	7400	0.412
3	14.127	22147	4654	0.197
4	15.230	294233	38561	2.614
5	15.637	45733	2576	0.406
6	15.954	28247	11872	0.251
7	16.119	10758656	1550369	95.590
8	18.312	18514	2192	0.164
Total		11255053	1623530	100.000