

Sample Name :Transportan
 Cat No.: RP20512
 Lot No.: E8217219L
 Time Processed :8:46:58
 Month-Day-Year Processed :12/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

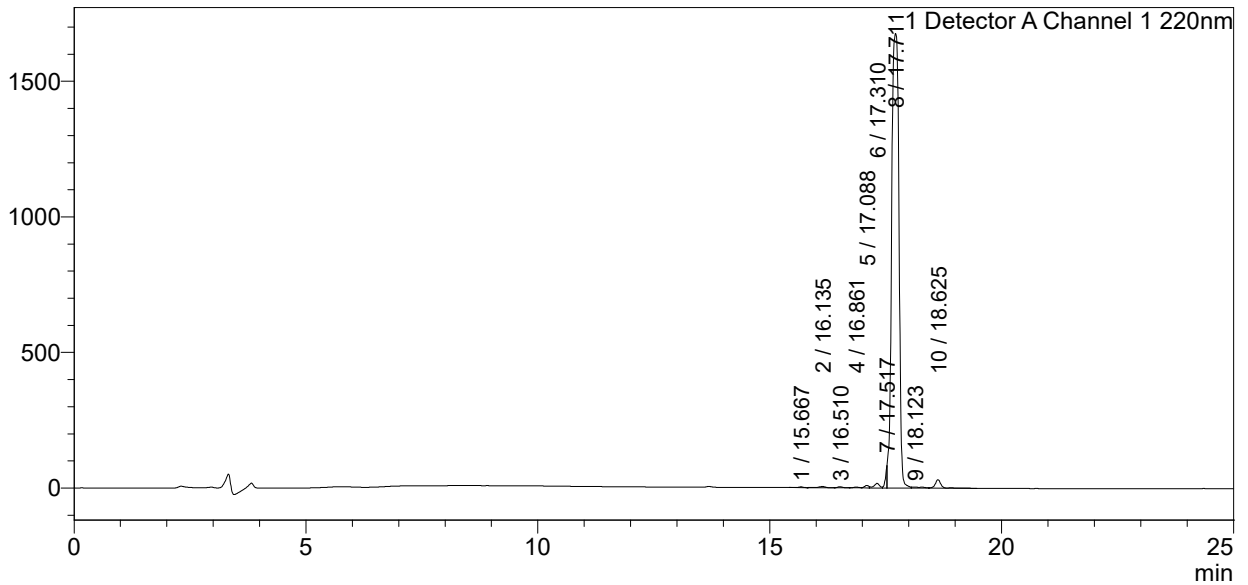

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.667	17469	2811	0.092
2	16.135	47155	4406	0.248
3	16.510	27568	4144	0.145
4	16.861	22834	3151	0.120
5	17.088	57294	9186	0.301
6	17.310	136621	16853	0.719
7	17.517	176318	68681	0.927
8	17.711	18179828	1676748	95.618
9	18.123	66273	3639	0.349
10	18.625	281673	31649	1.481
Total		19013032	1821269	100.000