


Mass Spectrum

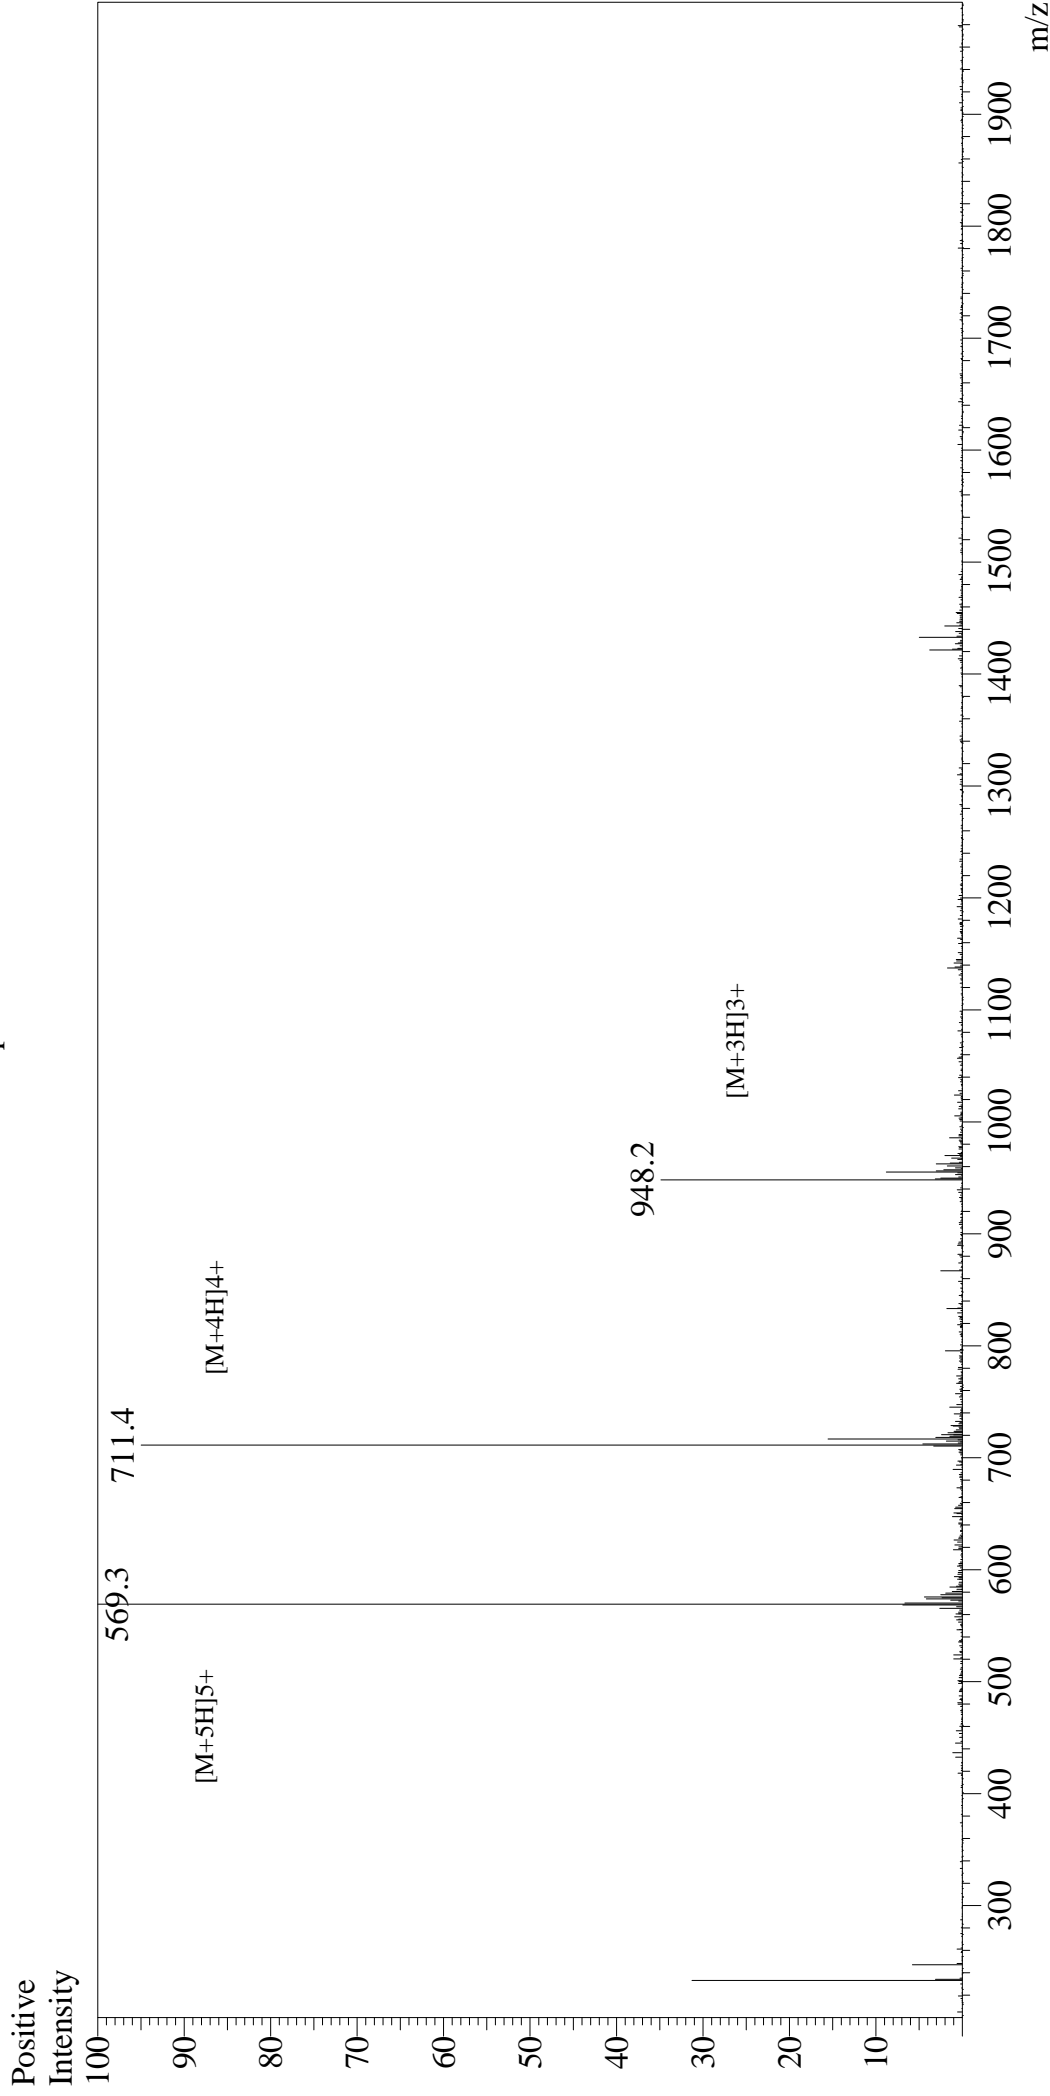

Sample Information

User : Gary
Month-Day Processed : 12/02/19
Time Processed : 20:11:57
Injection Volume : 0.3
Sample Name : Transportan
Cat No. : RP20512
Lot No. : E8217219L
Theoretical MW : 2841.50
Observed MW : 2841.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH