

Sample Name :Angiotensinogen (1-14), human

Cat. No. : RP10253

Lot. No. : E2668421D

Time Processed :11:08:30 PM

Month-Day-Year Processed :04/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

<Chromatogram>

mV

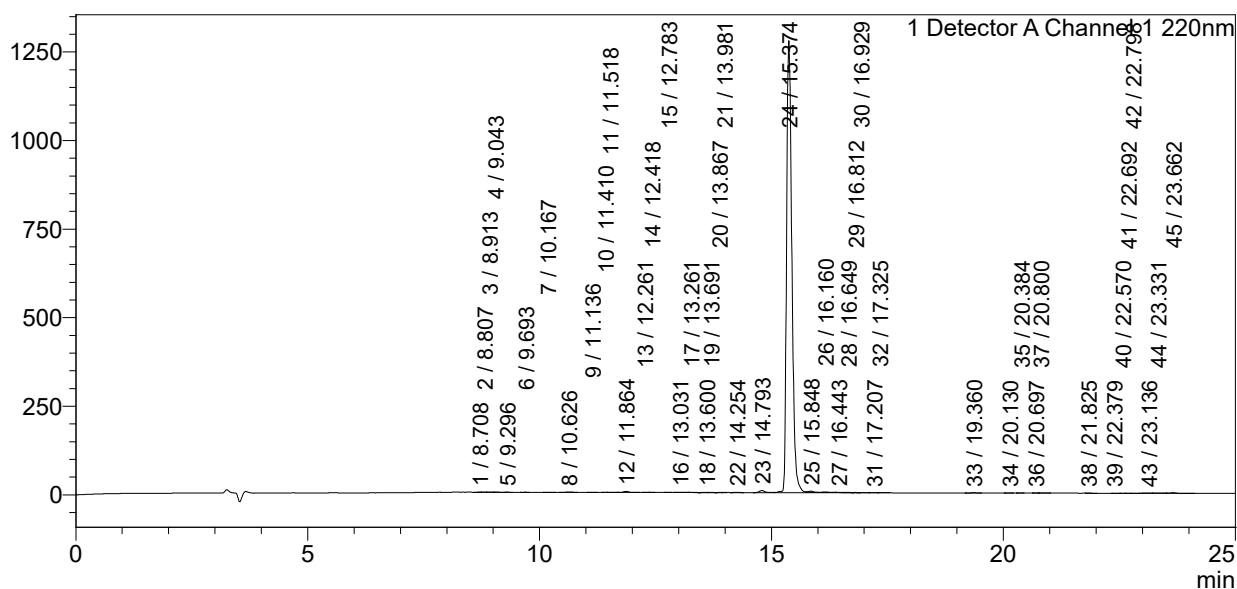

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.708	1337	259	0.013
2	8.807	2137	341	0.021
3	8.913	2991	348	0.029
4	9.043	1630	281	0.016
5	9.296	1573	268	0.015
6	9.693	1522	241	0.015
7	10.167	1877	276	0.018
8	10.626	7720	667	0.075
9	11.136	1847	275	0.018
10	11.410	1137	244	0.011
11	11.518	1920	228	0.019
12	11.864	22552	3158	0.218
13	12.261	1265	238	0.012
14	12.418	1061	253	0.010
15	12.783	1397	293	0.013
16	13.031	6212	793	0.060

Peak#	Ret. Time	Area	Height	Area%
17	13.261	2082	298	0.020
18	13.600	1148	190	0.011
19	13.691	1578	262	0.015
20	13.867	1337	211	0.013
21	13.981	1327	262	0.013
22	14.254	5020	722	0.048
23	14.793	51201	5919	0.494
24	15.374	10130057	1275919	97.786
25	15.848	16635	2536	0.161
26	16.160	10683	950	0.103
27	16.443	3401	369	0.033
28	16.649	2531	403	0.024
29	16.812	1286	290	0.012
30	16.929	1294	233	0.012
31	17.207	3963	537	0.038
32	17.325	3125	388	0.030
33	19.360	5490	756	0.053
34	20.130	1326	218	0.013
35	20.384	1241	228	0.012
36	20.697	1849	344	0.018
37	20.800	2369	345	0.023
38	21.825	1110	163	0.011
39	22.379	1882	243	0.018
40	22.570	1571	240	0.015
41	22.692	1471	289	0.014
42	22.798	2946	350	0.028
43	23.136	10827	827	0.105
44	23.331	11364	689	0.110
45	23.662	21099	2128	0.204
Total		10359389	1304470	100.000