

Sample Name :RGD  
 Cat No. : RP20297  
 Lot No. : E6251320  
 Time Processed :16:51:24  
 Month-Day-Year Processed :09/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

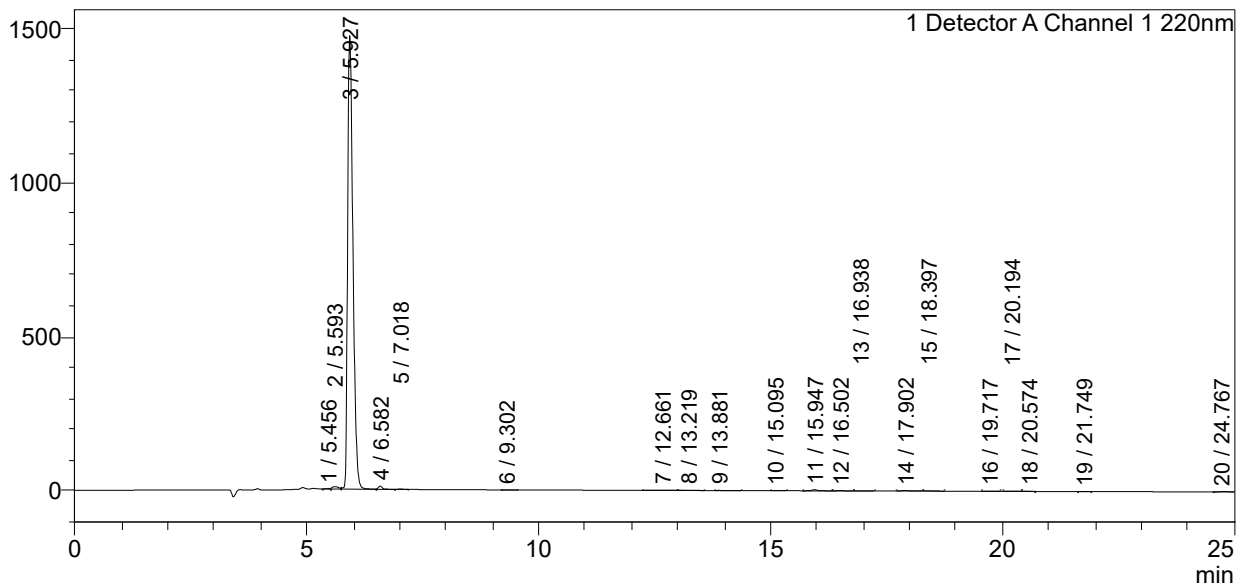

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.456	10733	1635	0.090
2	5.593	80257	7950	0.671
3	5.927	11698964	1477026	97.793
4	6.582	62558	10050	0.523
5	7.018	7724	983	0.065
6	9.302	1712	136	0.014
7	12.661	12967	594	0.108
8	13.219	4691	305	0.039
9	13.881	6609	287	0.055
10	15.095	1526	126	0.013
11	15.947	29861	3498	0.250
12	16.502	6507	788	0.054
13	16.938	2126	160	0.018
14	17.902	16396	1229	0.137
15	18.397	2665	162	0.022
16	19.717	2543	203	0.021

Peak#	Ret. Time	Area	Height	Area%
17	20.194	2106	184	0.018
18	20.574	2611	312	0.022
19	21.749	1032	134	0.009
20	24.767	9446	853	0.079
Total		11963034	1506617	100.000