

Sample Name :Arg-Gly-Asp-Cys
 Cat No. :RP10860
 Lot No. :E9047019G
 Time Processed :14:42:49
 Month-Day-Year Processed :07/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

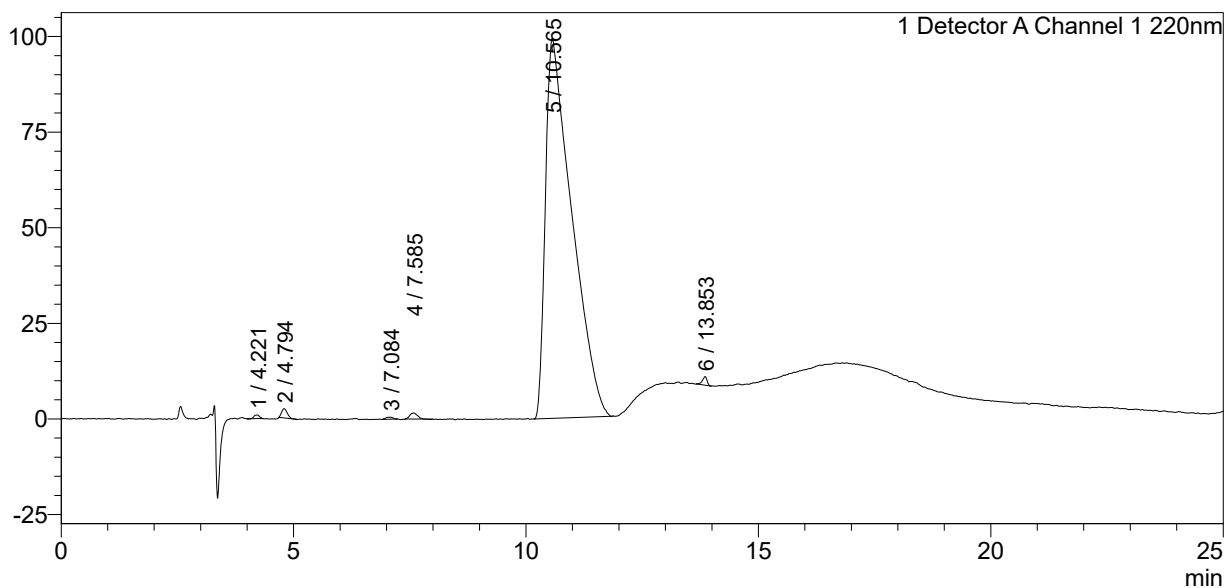

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.221	7739	960	0.194
2	4.794	20353	2436	0.511
3	7.084	5538	528	0.139
4	7.585	18264	1560	0.458
5	10.565	3918219	99372	98.312
6	13.853	15393	2279	0.386
Total		3985507	107135	100.000