

Sample Name : [Met<sup>5</sup>]-Enkephalin  
 Cat No.: RP10886 Lot No.: PE2091711  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

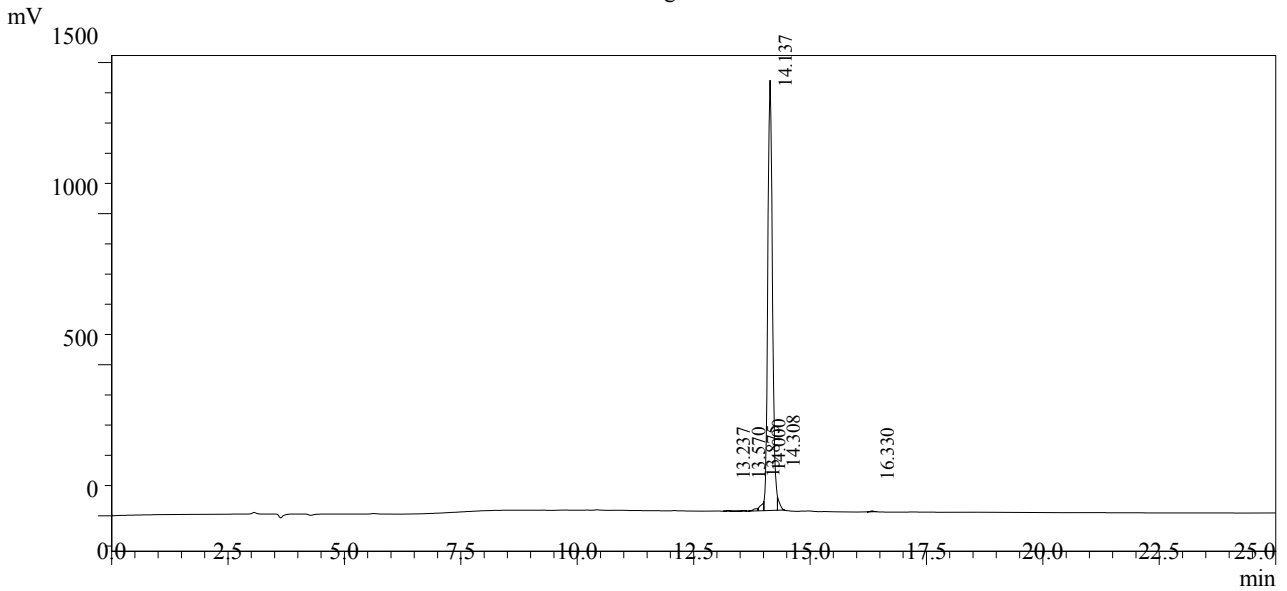

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.237	14363	2335	0.139
2	13.570	5568	1215	0.054
3	13.875	54311	7878	0.526
4	14.000	139707	26283	1.354
5	14.137	9954652	1423567	96.499
6	14.308	131520	40153	1.275
7	16.330	15735	2638	0.153
Total		10315856	1504068	100.000