

Sample Name :Ins B9-23  
 Cat. No. : RP20391  
 Lot. No. : E9616619L  
 Time Processed :13:31:56  
 Month-Day-Year Processed : 12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

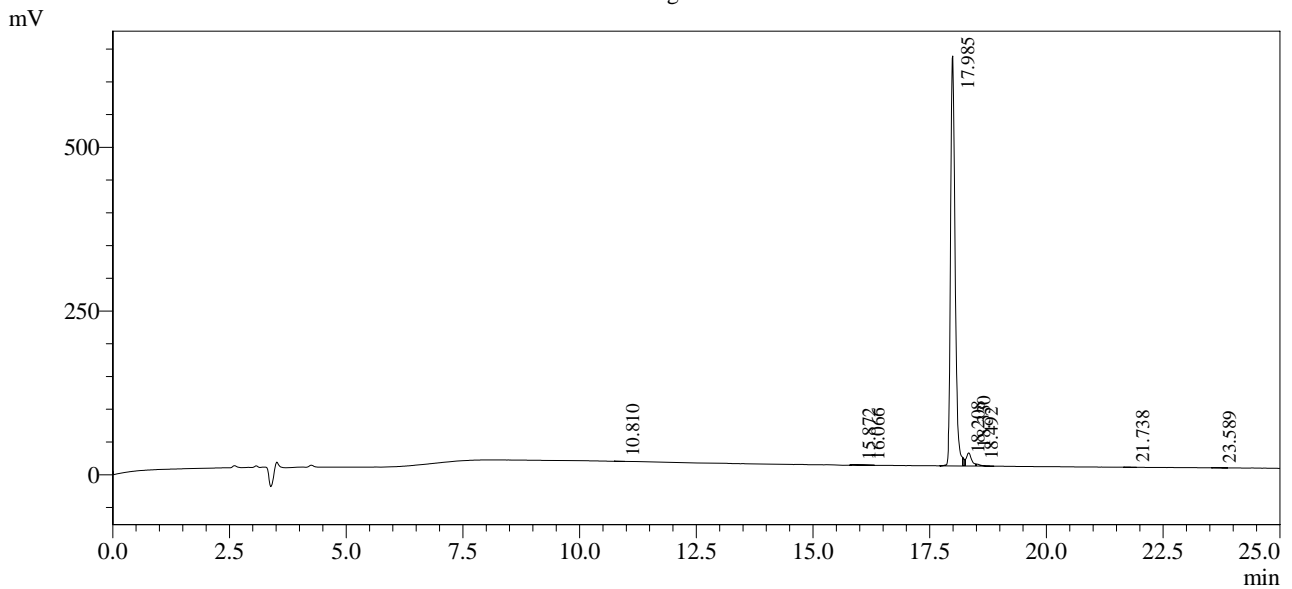

1 Det. A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.810	1879	392	0.042
2	15.872	4921	821	0.110
3	16.066	8065	779	0.181
4	17.985	4240947	626116	95.001
5	18.208	31916	12776	0.715
6	18.330	154079	19991	3.452
7	18.492	18774	3129	0.421
8	21.738	1777	275	0.040
9	23.589	1769	146	0.040
Total		4464127	664425	100.000