

Sample Name : SIYRY
 Cat. No. : RP20234
 Lot. No. : CB03907


Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

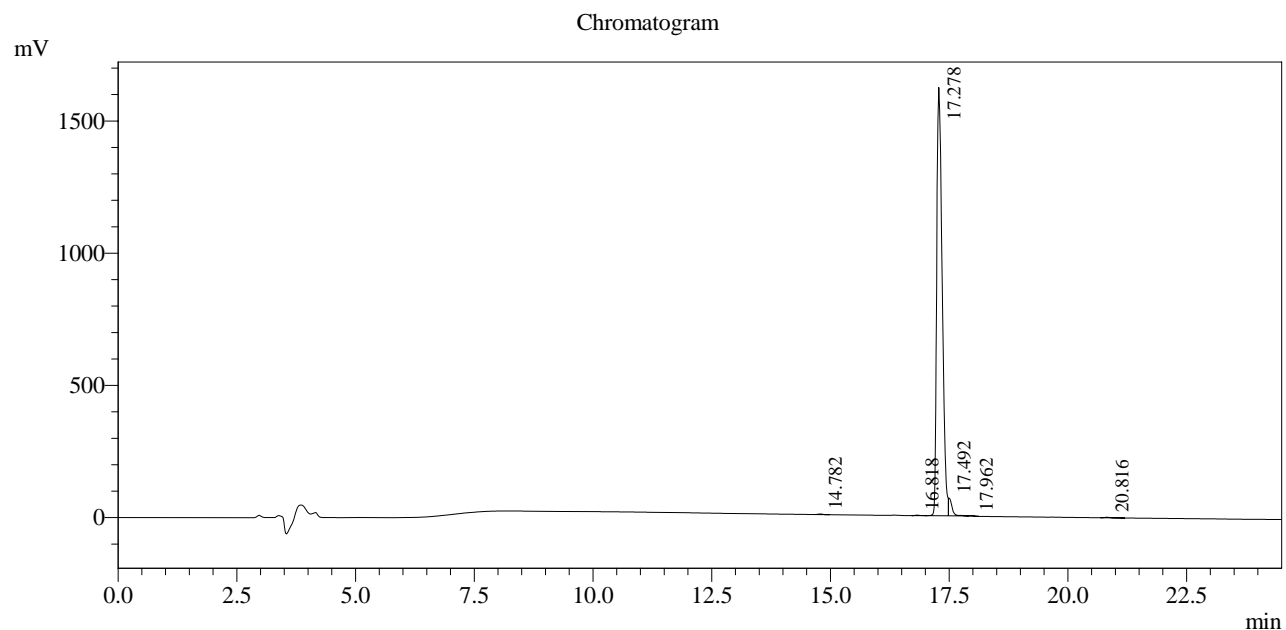

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	14.782	16982	2387	0.126
2	16.818	12262	1955	0.091
3	17.278	13123101	1620062	97.135
4	17.492	329465	66947	2.439
5	17.962	12590	2184	0.093
6	20.816	15814	2083	0.117
Total		13510216	1695618	100.000