

Sample Name : HIV gag199-207
 Cat. No. :RP20251
 Lot. No. :CD10907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

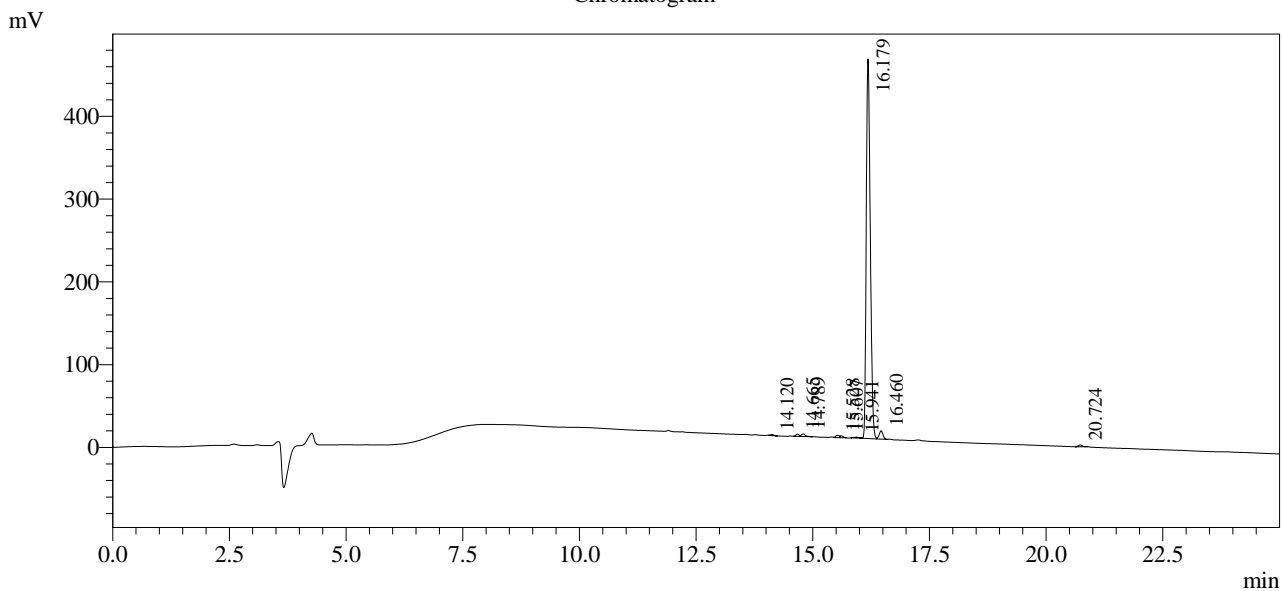

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	14.120	6120	1326	0.212
2	14.665	14008	2813	0.486
3	14.789	18593	3213	0.645
4	15.528	15466	2771	0.537
5	15.607	9322	2233	0.324
6	15.941	8948	1156	0.311
7	16.179	2742110	458848	95.163
8	16.460	55447	10060	1.924
9	20.724	11477	2119	0.398
Total		2881490	484540	100.000