

Sample Name : PAR-4 Agonist,amide,murine
 Cat. No. :RP20296
 Lot. No. :CD12907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

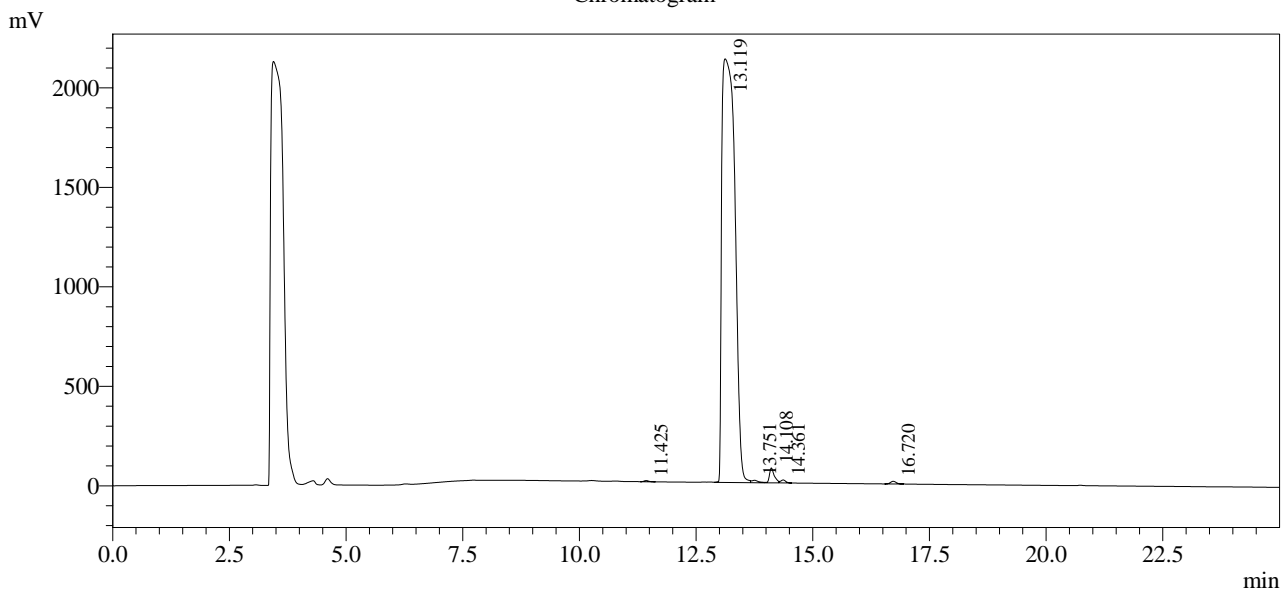

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	11.425	39468	5924	0.093
2	13.119	41646564	2129247	97.818
3	13.751	125089	12348	0.294
4	14.108	538530	75027	1.265
5	14.361	112115	14912	0.263
6	16.720	113824	13430	0.267
Total		42575590	2250888	100.000