

Sample Name : RGD
 Cat. No. : RP20297
 Lot. No. : CC04907


Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

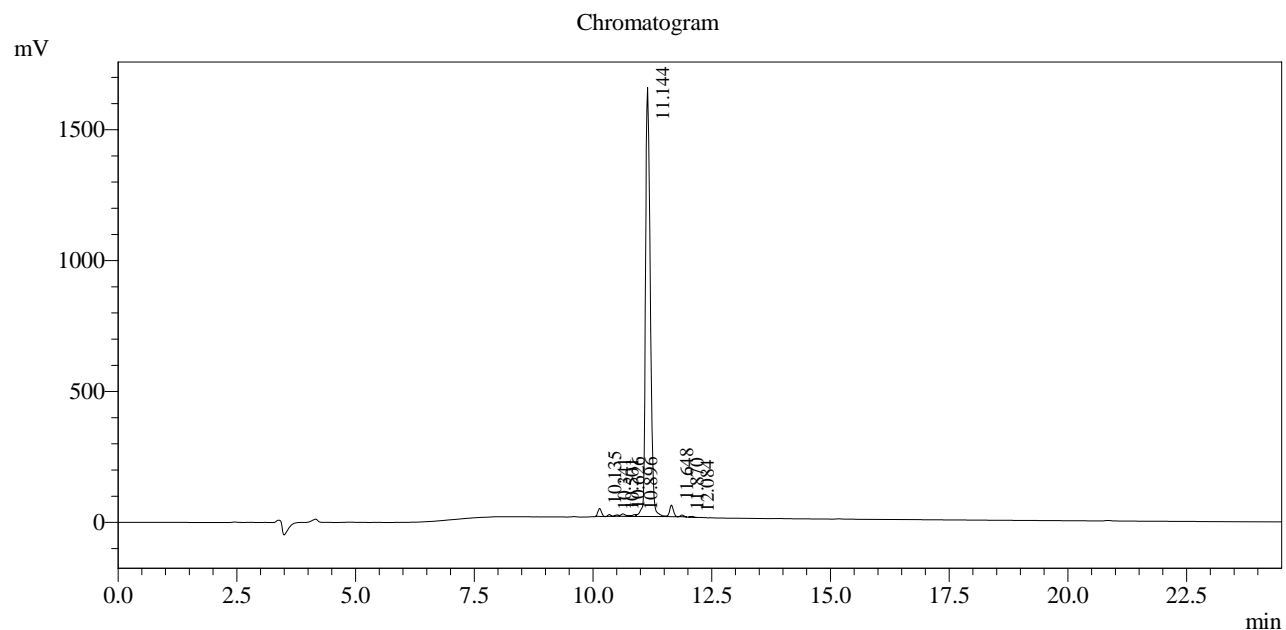

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	10.135	156044	30648	1.287
2	10.341	28893	6881	0.238
3	10.501	27313	5218	0.225
4	10.626	71469	9226	0.590
5	10.896	37635	7773	0.311
6	11.144	11514727	1639045	95.005
7	11.648	242095	44153	1.997
8	11.870	29985	6418	0.247
9	12.084	11984	2526	0.099
Total		12120144	1751889	100.000