


Positive

MS Spectrum

Intensity

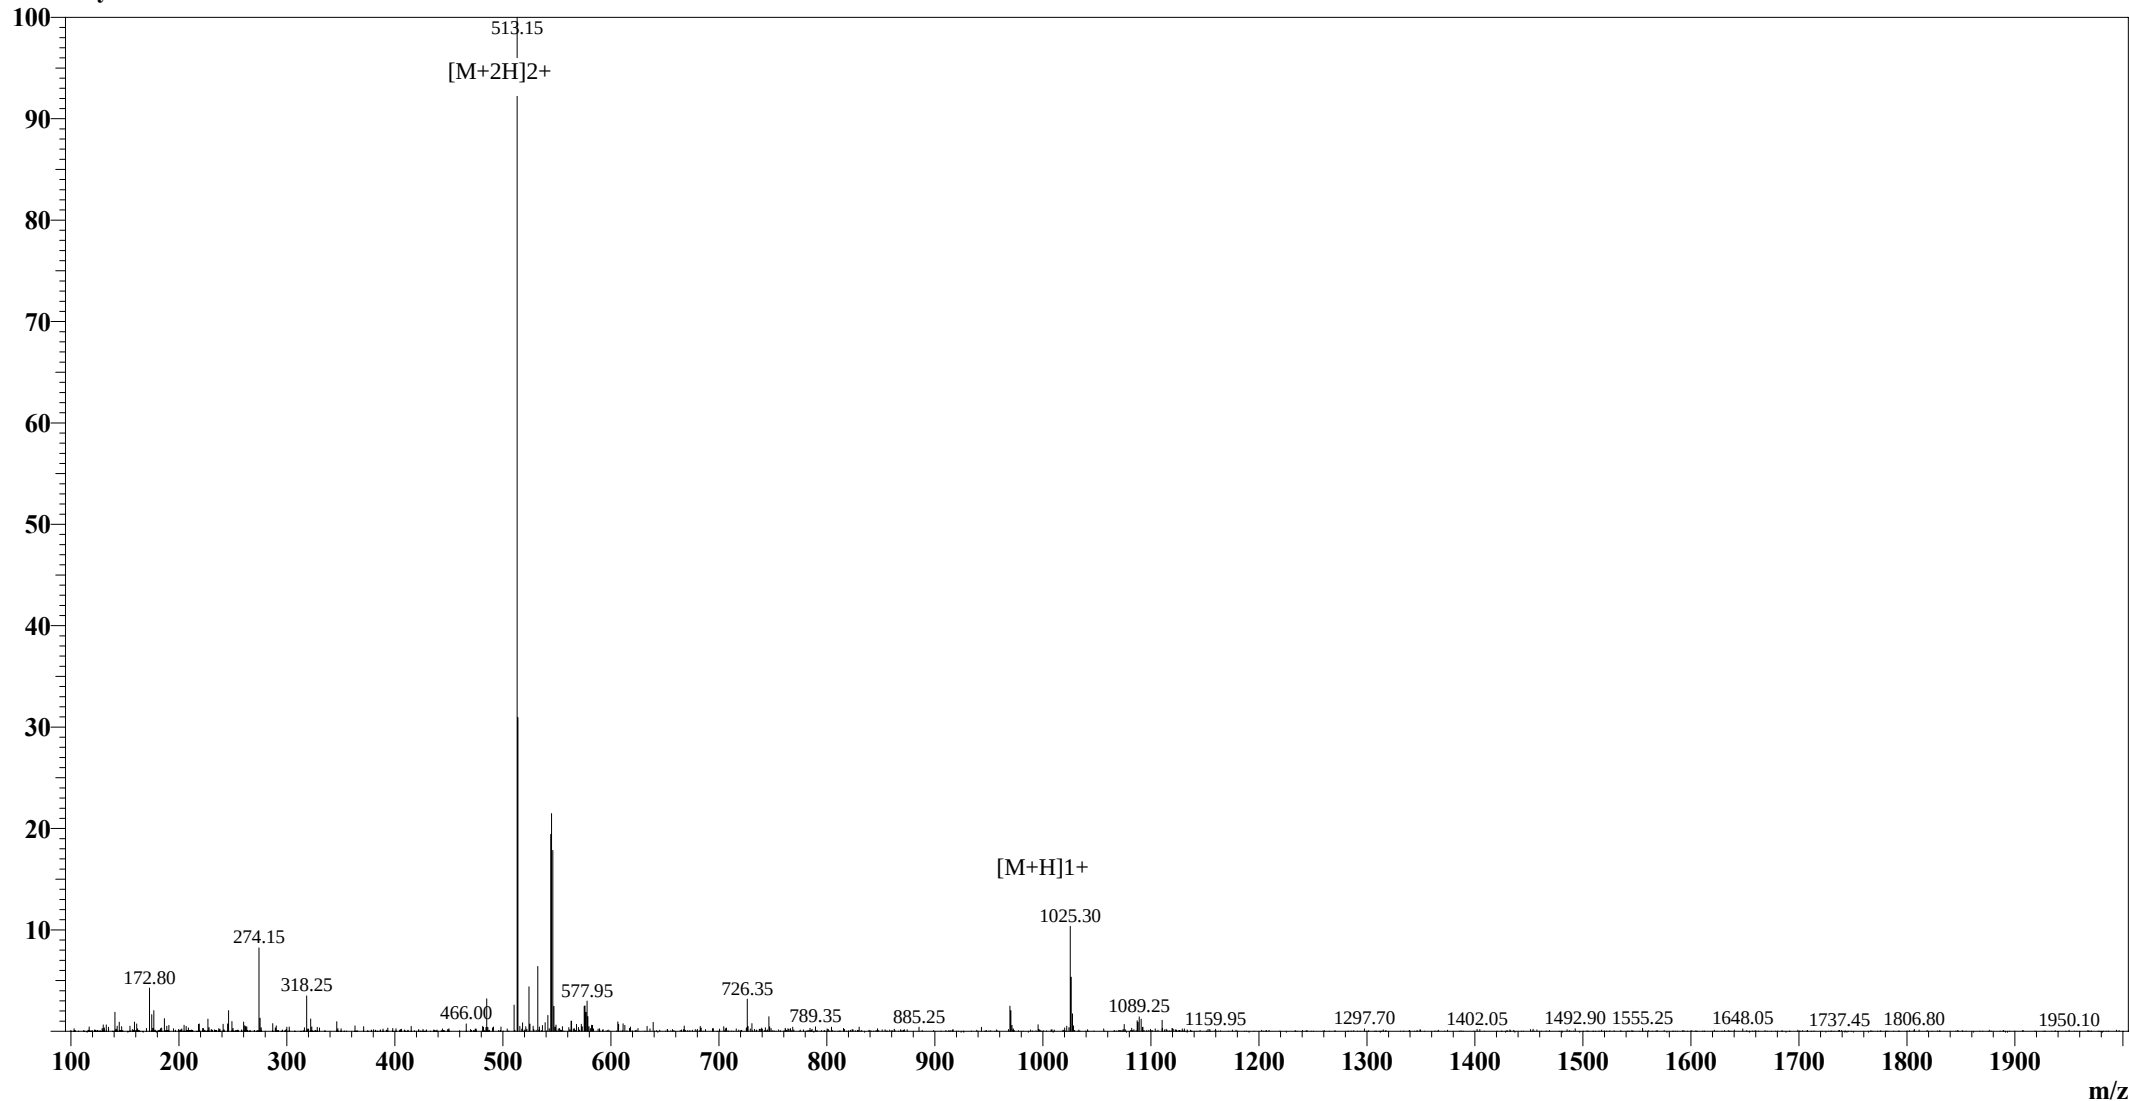

Sample Information

User : Grace
Date Acquired : 07/07/2009 21:25:15
Sample Name : RGD
Cat No. : RP20297
Lot No. : CC04907
Injection Volum : 1.000µL
Theoretical MW : 1024.06
Observed MW : 1024.30

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH