

Sample Name : p5
 Cat. No. : RP20327
 Lot. No. : CC07907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
45.00	Pumps	Pump B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

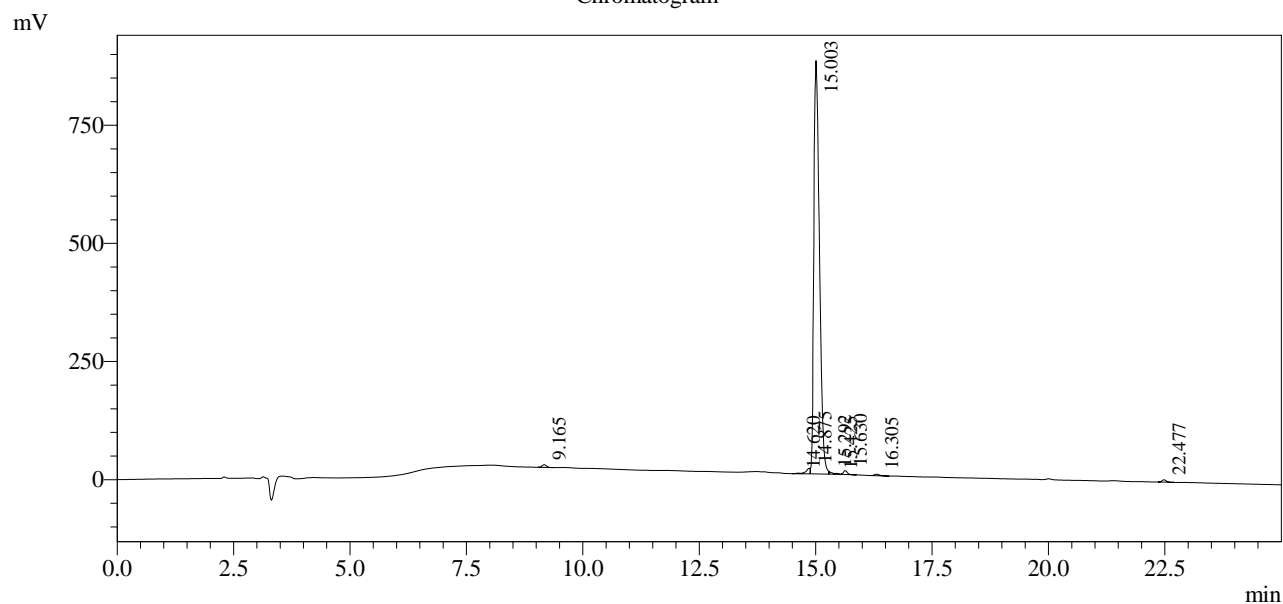

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	9.165	38571	5698	0.508
2	14.620	7642	1208	0.101
3	14.875	70263	11820	0.926
4	15.003	7340085	874696	96.727
5	15.292	22960	5015	0.303
6	15.425	5699	1664	0.075
7	15.630	48140	8224	0.634
8	16.305	23723	3165	0.313
9	22.477	31368	4994	0.413
Total		7588451	916484	100.000