

Sample Name : IRBP (1 - 20), human
 Cat. No. : RP20269
 Lot. No. : CA15907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

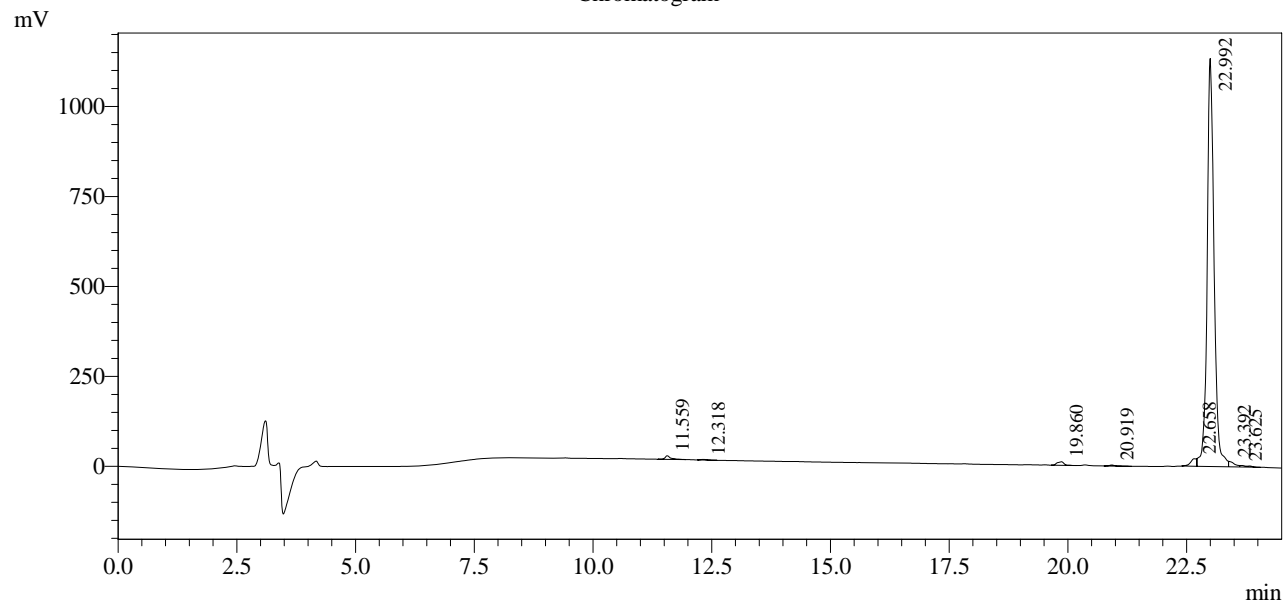

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	11.559	81041	9795	0.671
2	12.318	12986	1735	0.108
3	19.860	100471	10108	0.832
4	20.919	23810	2819	0.197
5	22.658	187133	20581	1.550
6	22.992	11496323	1133901	95.200
7	23.392	125099	14768	1.036
8	23.625	49118	4016	0.407
Total		12075980	1197724	100.000