

Sample Name : Influenza NP (147-155)
 Cat. No. :RP20260
 Lot. No. :CC10907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

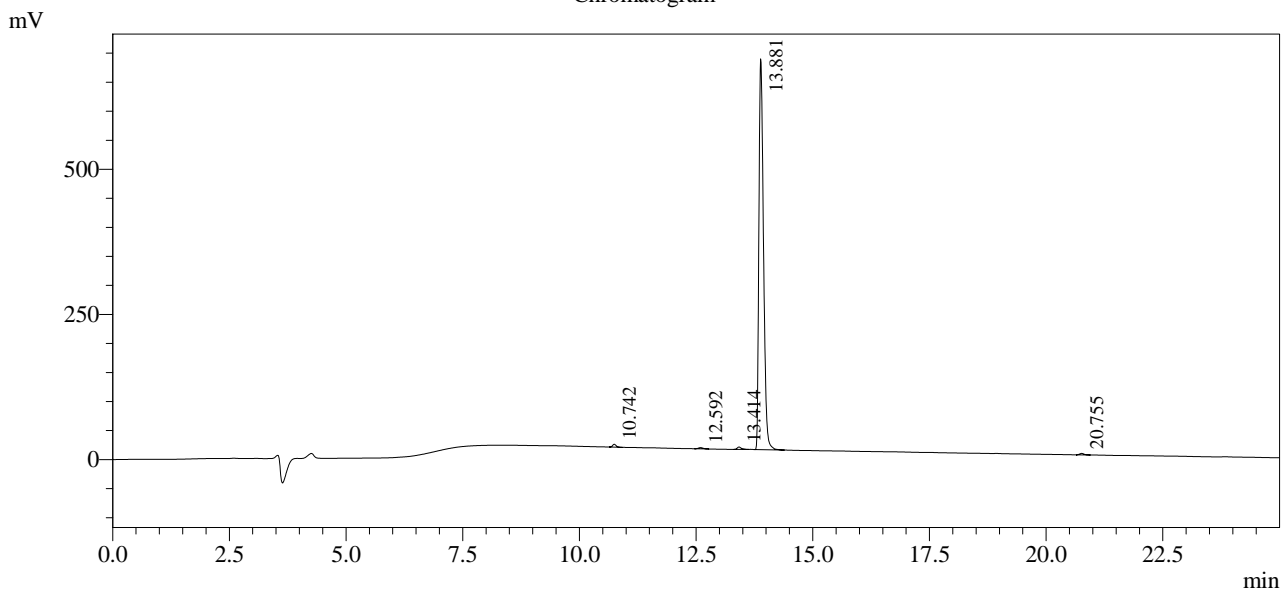

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	10.742	25747	4927	0.548
2	12.592	14757	2136	0.314
3	13.414	26531	4212	0.564
4	13.881	4617486	673093	98.229
5	20.755	16220	2577	0.345
Total		4700742	686945	100.000