

Sample Name : ACTH(1-39),rat
Cat. No. :RP11305
Lot. No. :CC11907

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

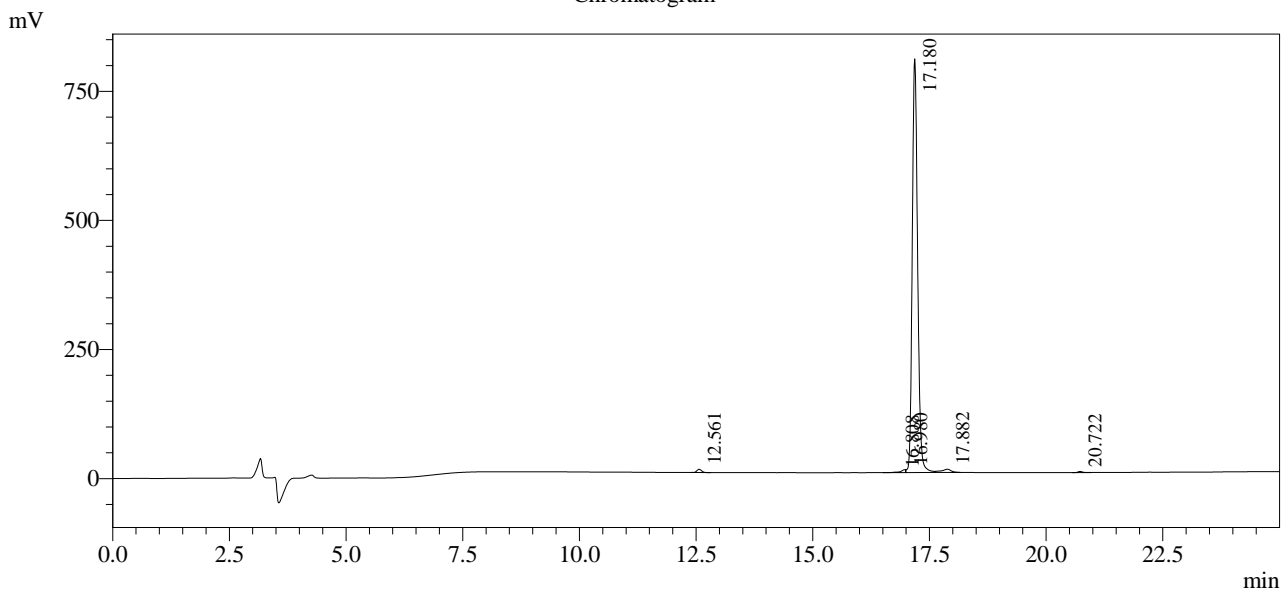

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.561	44122	6360	0.668
2	16.808	7748	1076	0.117
3	16.980	35854	5644	0.543
4	17.180	6407410	801274	97.056
5	17.882	91777	6281	1.390
6	20.722	14838	2193	0.225
Total		6601749	822828	100.000