


Positive

MS Spectrum

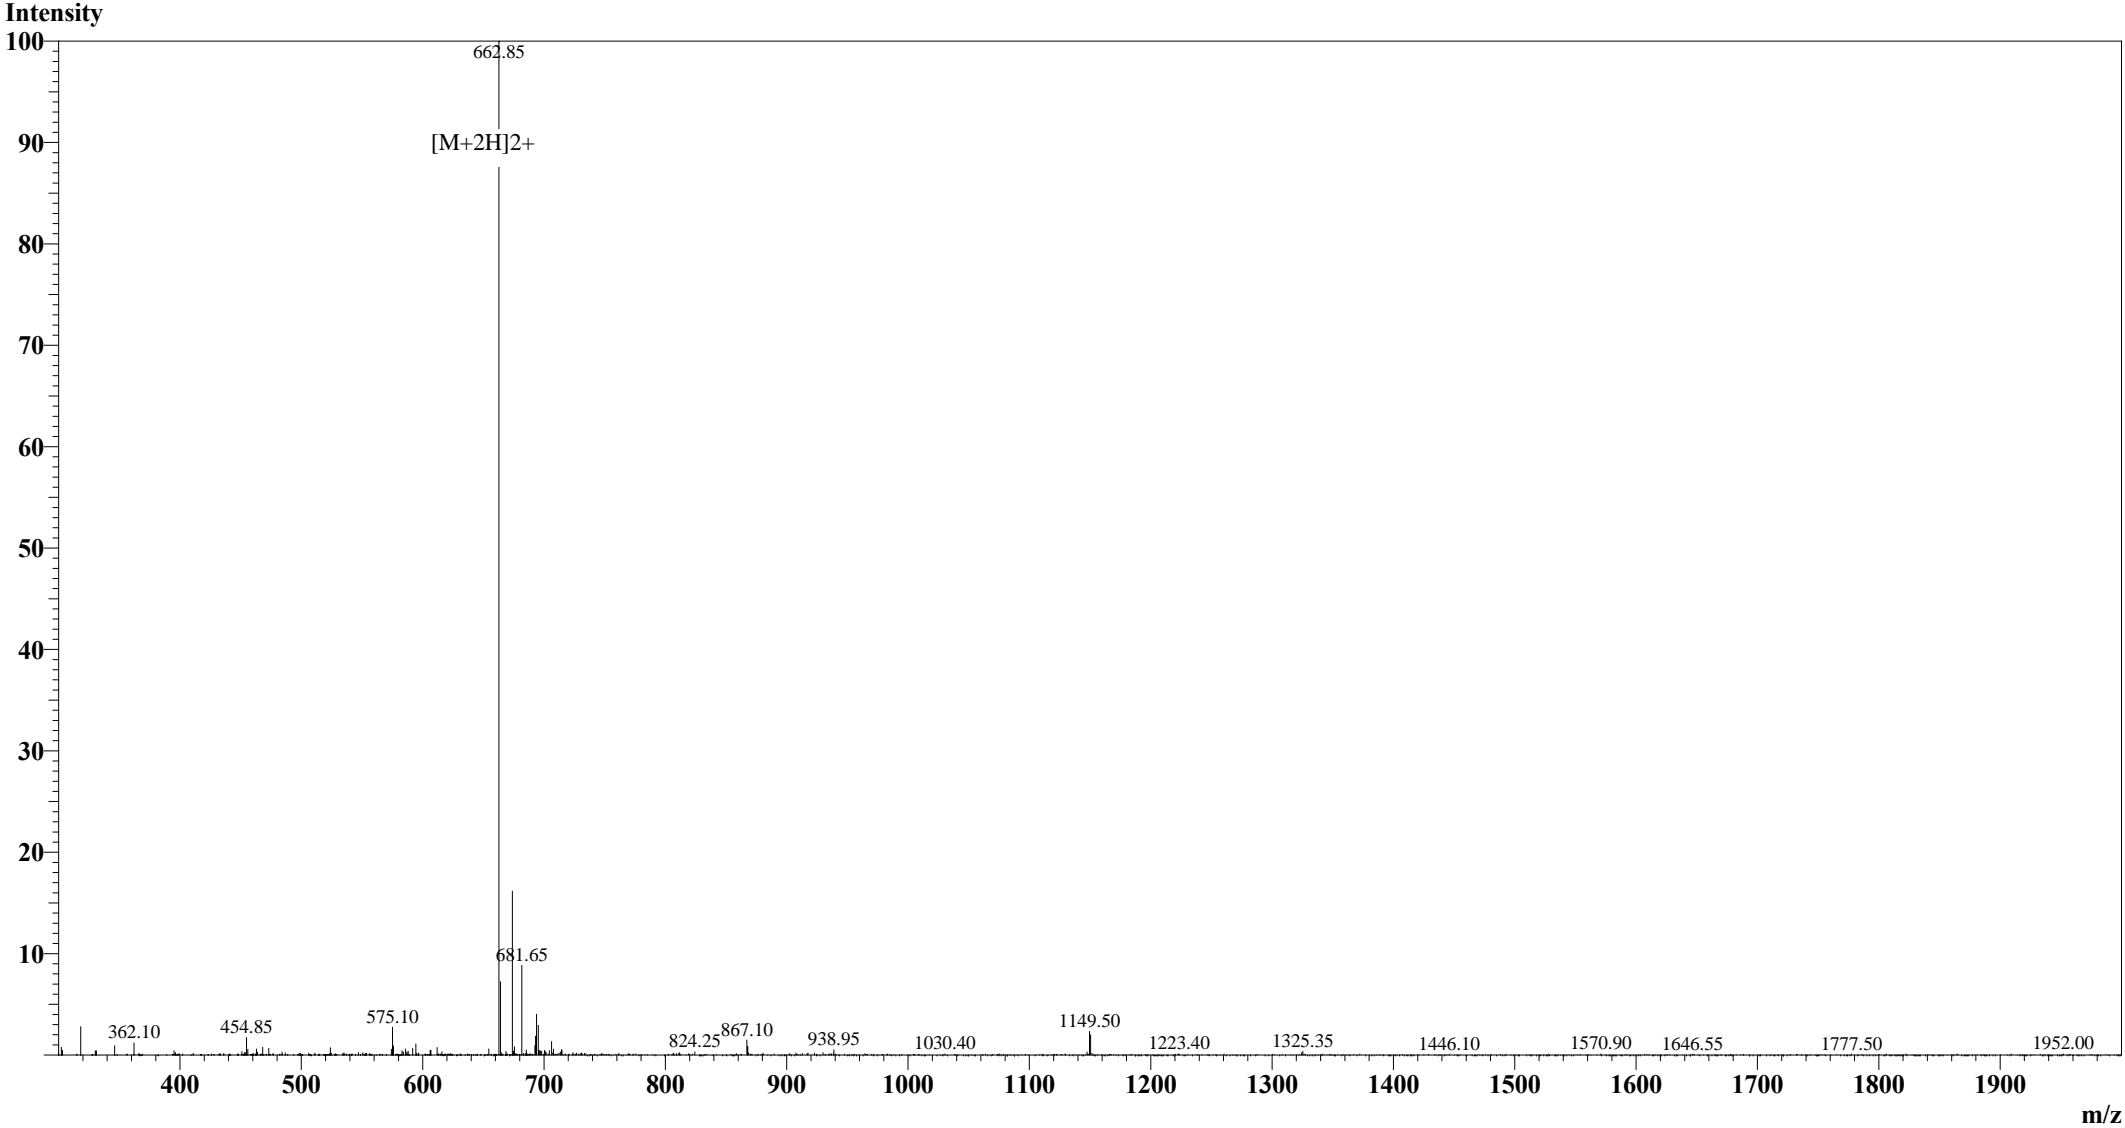

Sample Information					
User	:Grace	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	: 08/23/2009 10:05:09	Nebulizing Gas Flow	:1.50 L/min	Detector	:1.5kv
Sample Name	:HA-(126-138)	CDL Temp	: 250°C	T.Flow	: 0.2ml/min
Cat No.	: RP20240	CDL Volt	: -25.0V	B.conc	: 50%H2O/50%MeOH
Lot No.	: CC05908	Block Temp	: 200°C		
Injection Volum	: 1.000µL				
Theoretical MW	: 1324.34				
Observed MW	:1323.70				