

Sample Name : MARK substrate
 Cat. No. : RP20244
 Lot. No. : CA08908

Pump A : 0.065% trifluoroacetic in 100% water

Pump B : 0.05% trifluoroacetic in 100% acetonitrile

Total Flow : 1 ml / min


Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

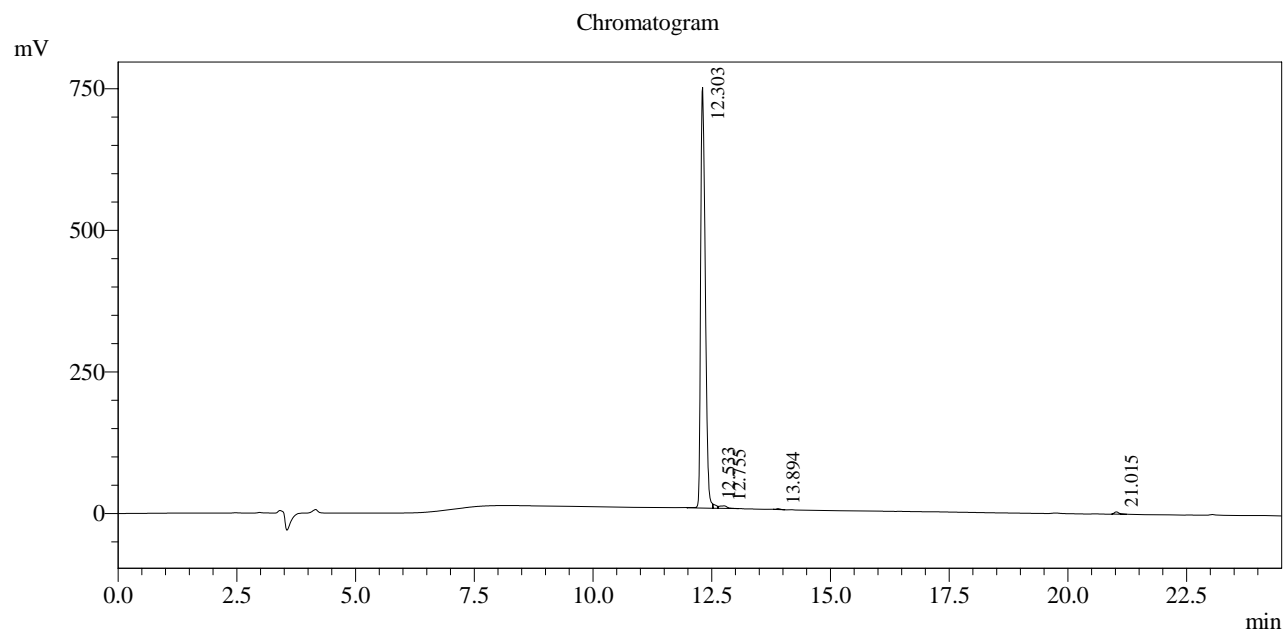

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.303	4996440	742596	97.662
2	12.533	33550	7010	0.656
3	12.755	50458	4535	0.986
4	13.894	8792	1600	0.172
5	21.015	26820	3987	0.524
Total		5116060	759728	100.000