

Sample Name : WKYMVm
 Cat. No. : RP20299
 Lot. No. : CD12908

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

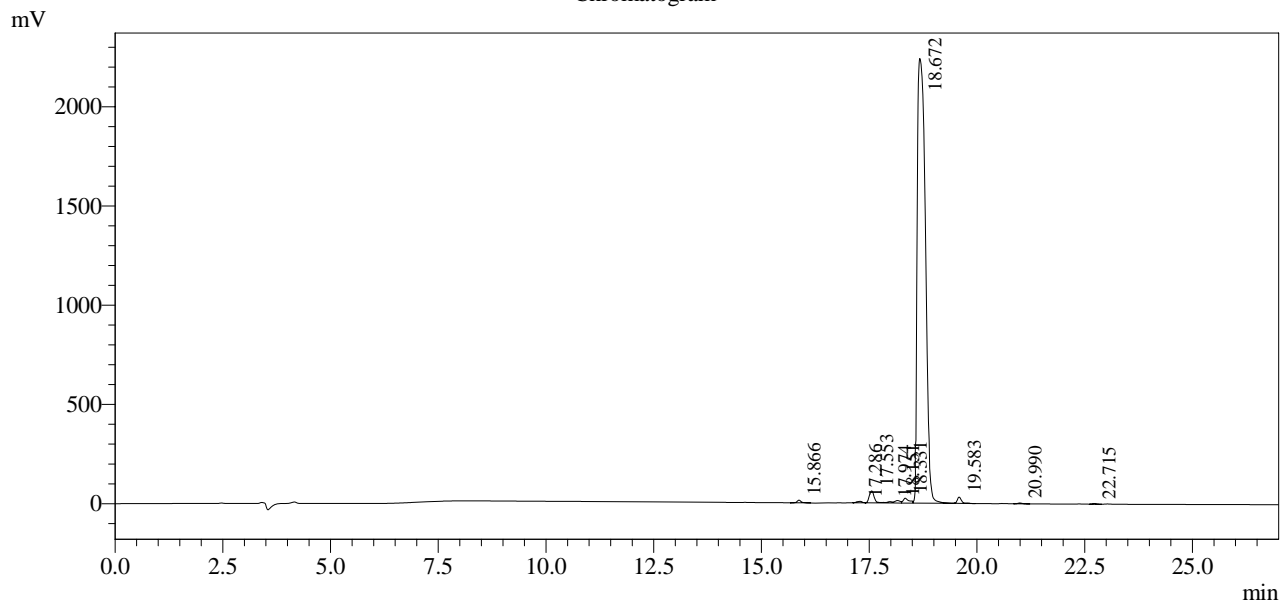

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.866	81598	13360	0.264
2	17.286	66270	7661	0.215
3	17.553	488634	60364	1.584
4	17.974	52559	6703	0.170
5	18.151	110321	12515	0.358
6	18.331	231310	24504	0.750
7	18.672	29558628	2240647	95.800
8	19.583	218438	31642	0.708
9	20.990	29793	4191	0.097
10	22.715	16898	2745	0.055
Total		30854449	2404331	100.000