

Sample Name : Casein Kinase Substrates 3
 Cat. No. : RP20214
 Lot. No. : CB03908

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min


Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

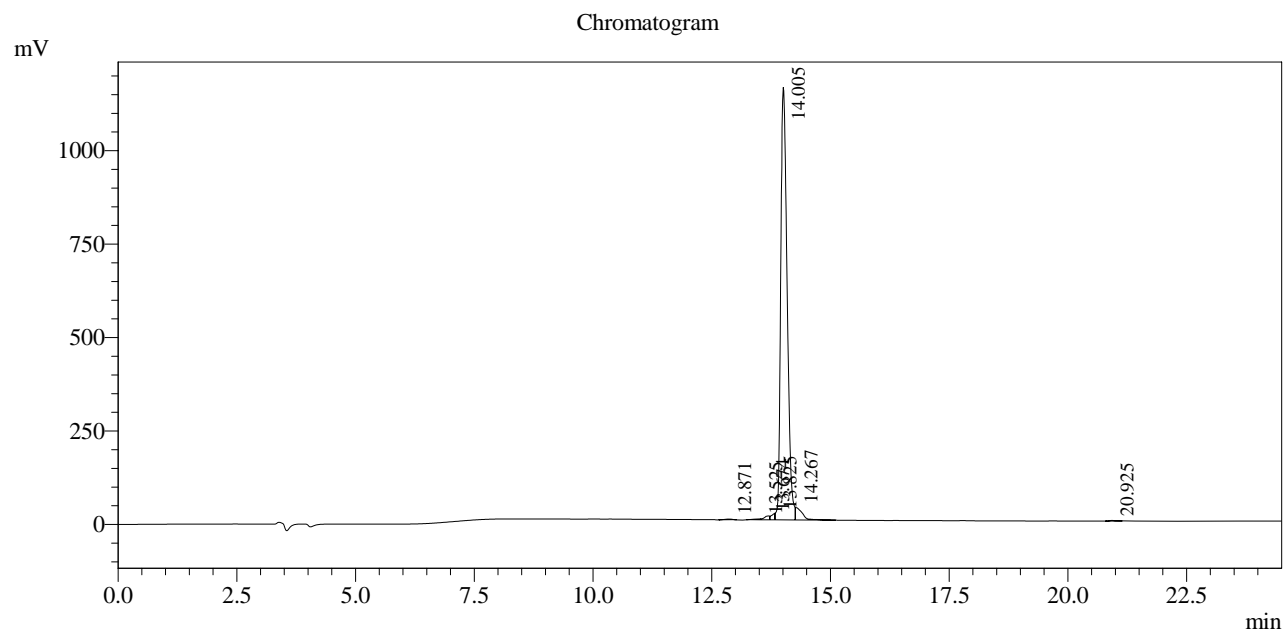

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.871	16474	1747	0.144
2	13.525	22270	2283	0.195
3	13.674	80947	10385	0.707
4	13.825	89111	17346	0.778
5	14.005	10885788	1157106	95.090
6	14.267	338316	33423	2.955
7	20.925	14935	1915	0.130
Total		11447840	1224205	100.000