

Sample Name : AGT(1-14),human  
 Cat. No. : RP20216  
 Lot. No. : CC02908


Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow : 1 ml / min  
 Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

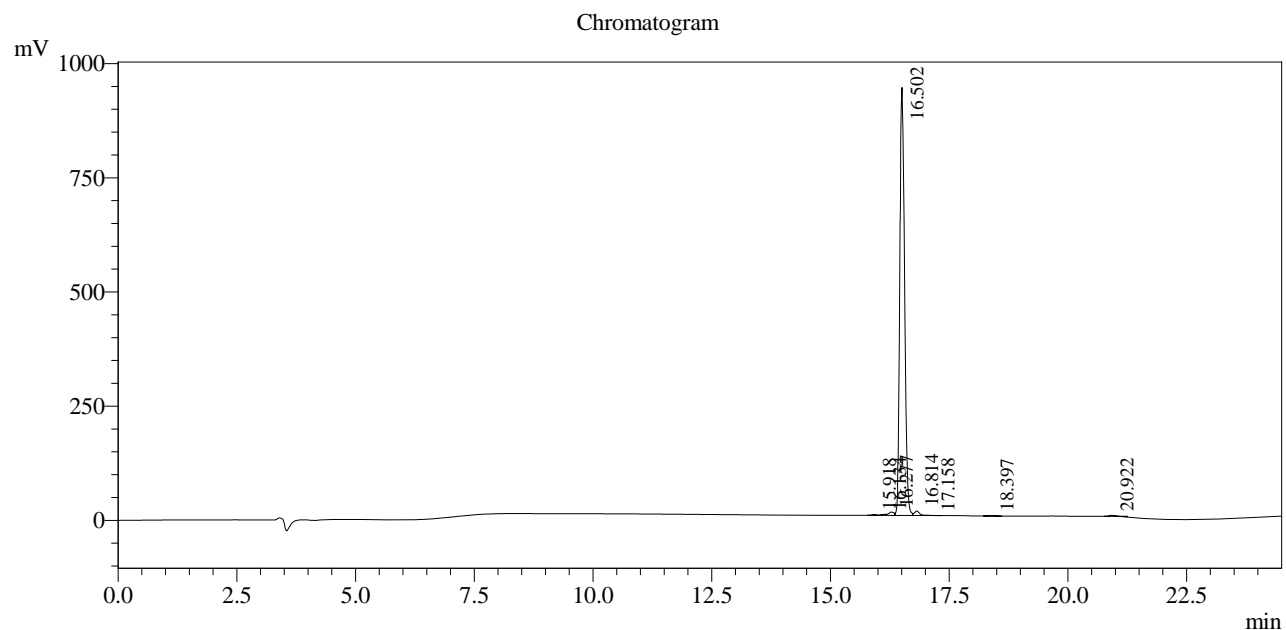

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.918	10907	1476	0.160
2	16.134	15280	2239	0.224
3	16.277	58181	7364	0.854
4	16.502	6630296	937062	97.305
5	16.814	74055	9822	1.087
6	17.158	4376	529	0.064
7	18.397	3548	573	0.052
8	20.922	17309	2053	0.254
Total		6813952	961118	100.000