

Sample Name : TFLLR-NH2
 Cat. No. :RP20354
 Lot. No. :CD09909

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

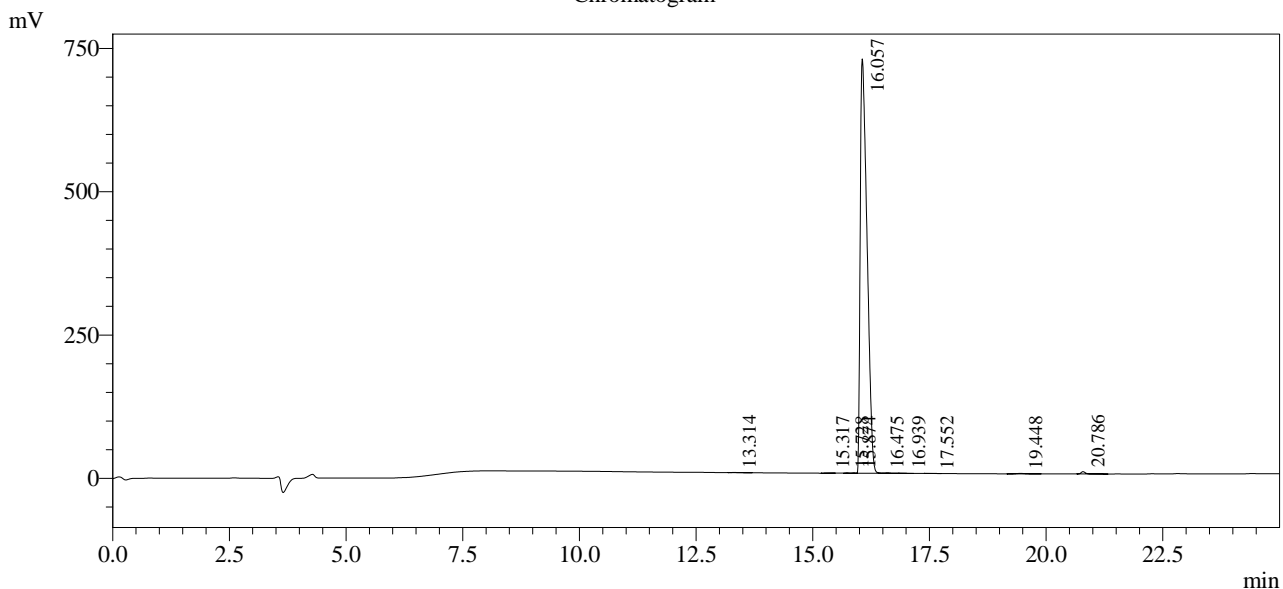

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.314	2586	304	0.035
2	15.317	446	98	0.006
3	15.728	2614	461	0.035
4	15.874	2660	473	0.036
5	16.057	7345424	723059	99.324
6	16.475	3087	351	0.042
7	16.939	1147	172	0.016
8	17.552	2089	246	0.028
9	19.448	8285	735	0.112
10	20.786	27093	4008	0.366
Total		7395430	729910	100.000