

Sample Name : HIV - 1 Rev (34 - 50)  
 Cat. No. : RP20362  
 Lot. No. : CA10909

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile

Total Flow : 1 ml / min


Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

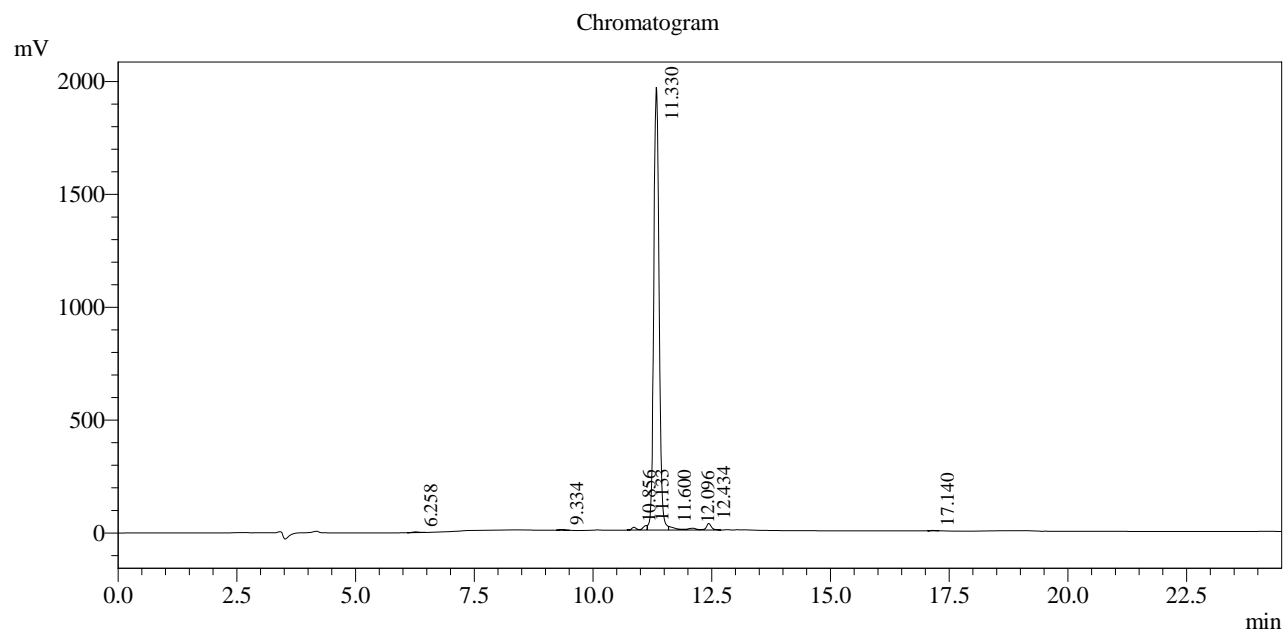

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.258	30270	3232	0.187
2	9.334	17865	2677	0.111
3	10.856	87193	12798	0.540
4	11.133	115551	19959	0.715
5	11.330	15444307	1960780	95.562
6	11.600	148599	14953	0.919
7	12.096	93884	7839	0.581
8	12.434	212477	28634	1.315
9	17.140	11464	1910	0.071
Total		16161611	2052783	100.000