

Sample Name : HEX3
 Cat. No. :RP20346
 Lot. No. :CD15909

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

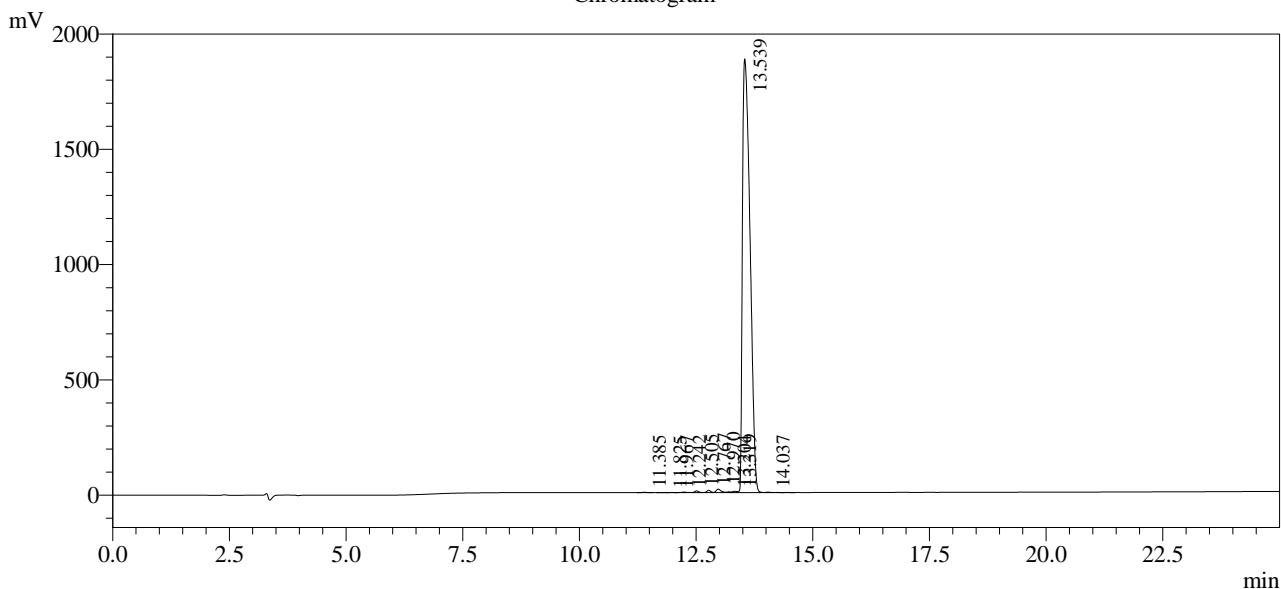

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.385	10245	1555	0.048
2	11.825	717	70	0.003
3	11.967	3210	511	0.015
4	12.242	18696	2238	0.087
5	12.505	47482	7454	0.220
6	12.767	59863	10130	0.278
7	12.970	109449	15137	0.508
8	13.204	17259	3218	0.080
9	13.319	34020	5698	0.158
10	13.539	21221504	1880910	98.536
11	14.037	14296	1763	0.066
Total		21536740	1928683	100.000