

Sample Name : Fibronectin Active Fragment Control
 Cat. No. : RP20347
 Lot. No. : CA14909

Pump A : 0.065% trifluoroacetic in 100% water

Pump B : 0.05% trifluoroacetic in 100% acetonitrile

Total Flow : 1 ml / min

Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

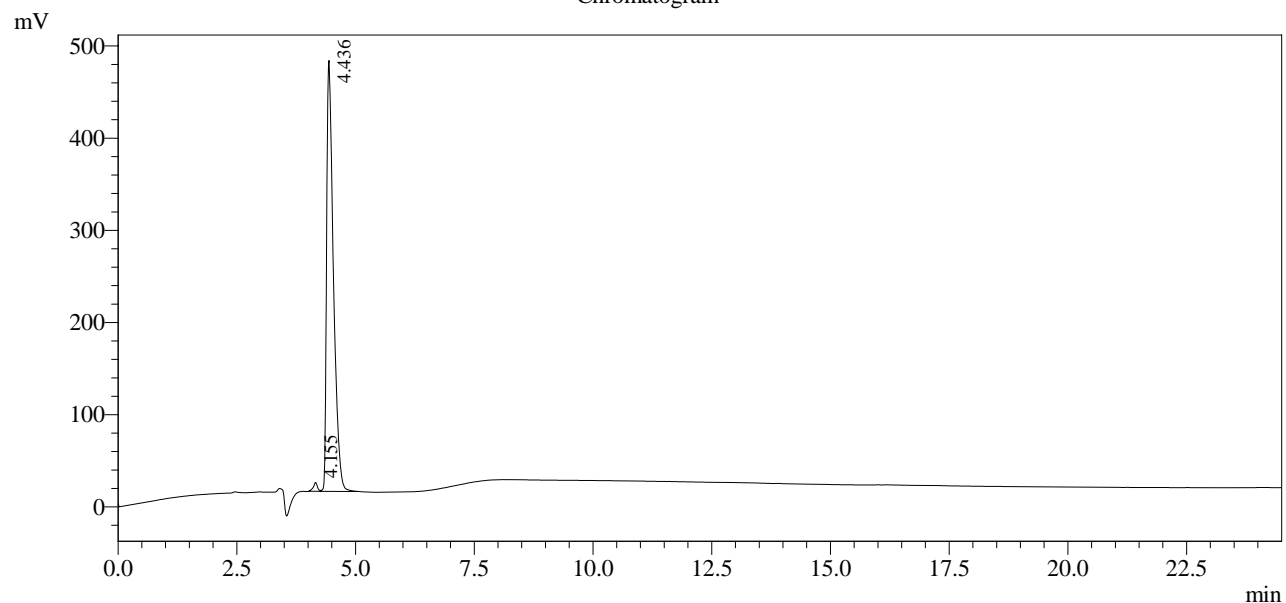

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.155	57677	9690	1.222
2	4.436	4660842	467474	98.778
Total		4718520	477164	100.000