

Sample Name :ANP(1-28)
Cat. No. :RP11927
Lot. No. :CC06910

Pump A : 0.065% trifluoroacetic in 100% water
Pump B : 0.05% trifluoroacetic in 100% acetonitrile
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

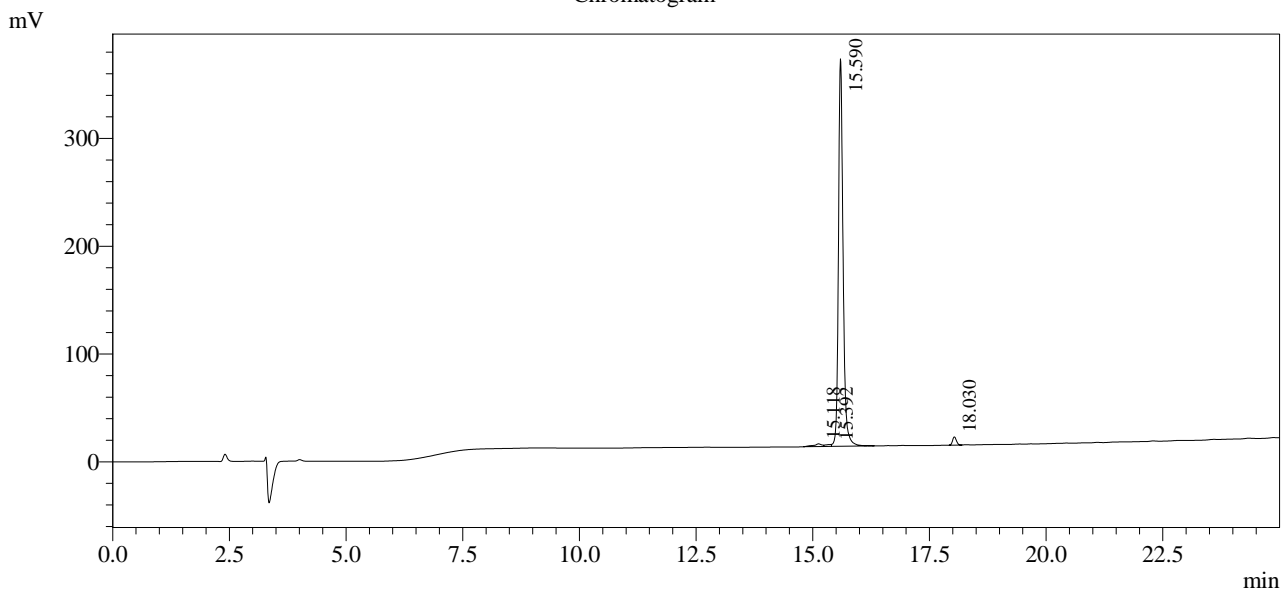

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.118	31362	2490	1.218
2	15.392	15513	1735	0.602
3	15.590	2484178	359411	96.477
4	18.030	43833	7652	1.702
Total		2574886	371287	100.000